

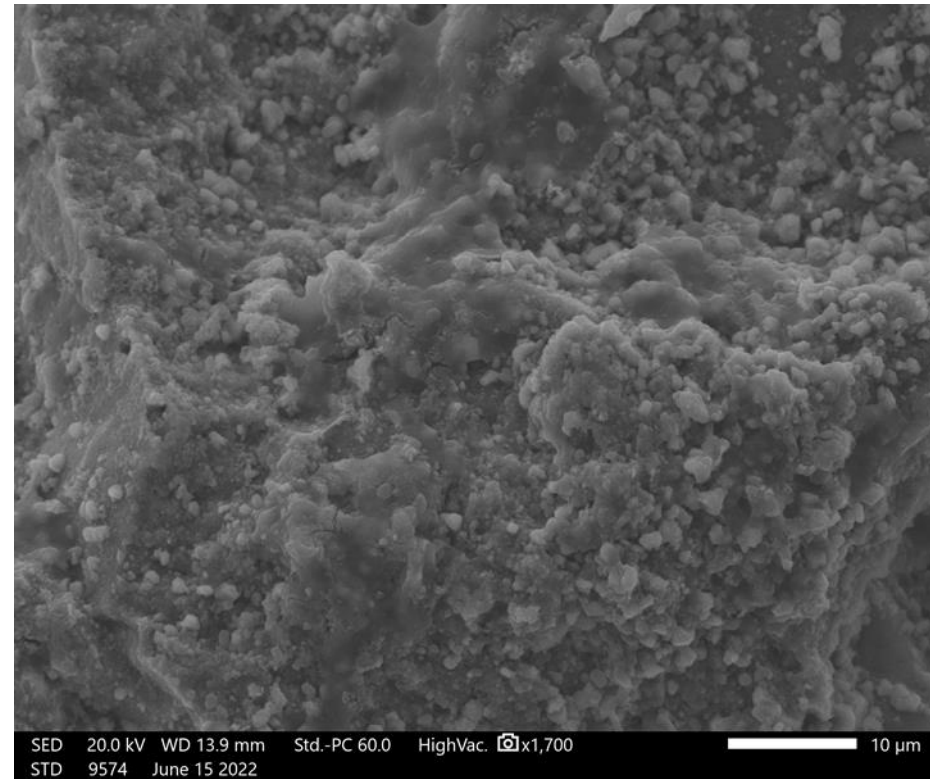



ΠΑΡΑΡΤΗΜΑ IV- ΦΩΤΟΓΡΑΦΙΕΣ SEM

ΚΑΤΗΓΟΡΙΑ Ι (ΔΟΚΙΜΙΑ ΑΝΑΦΟΡΑΣ)

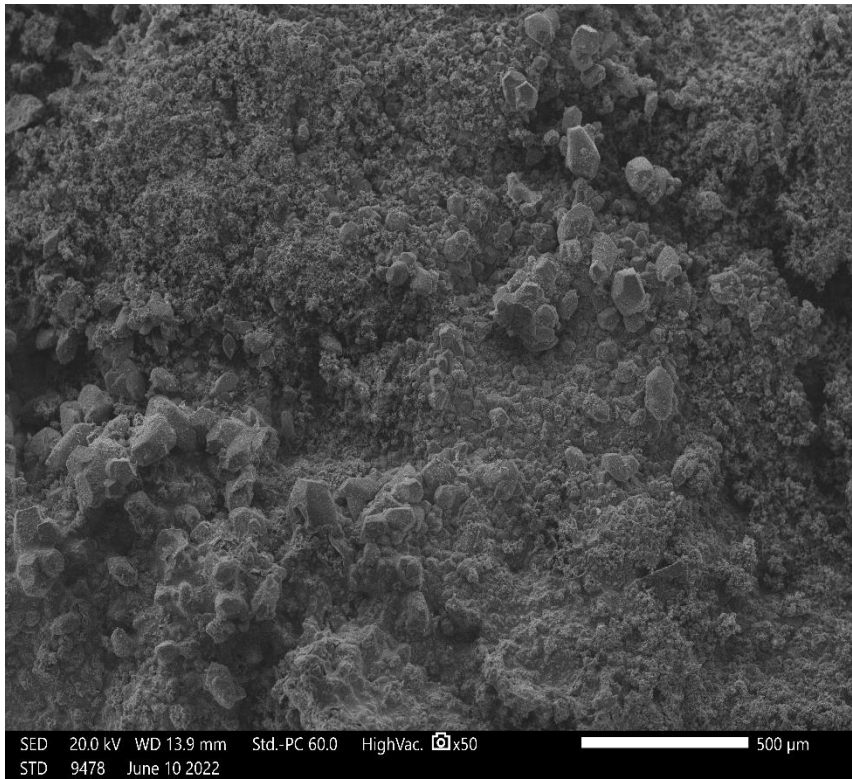


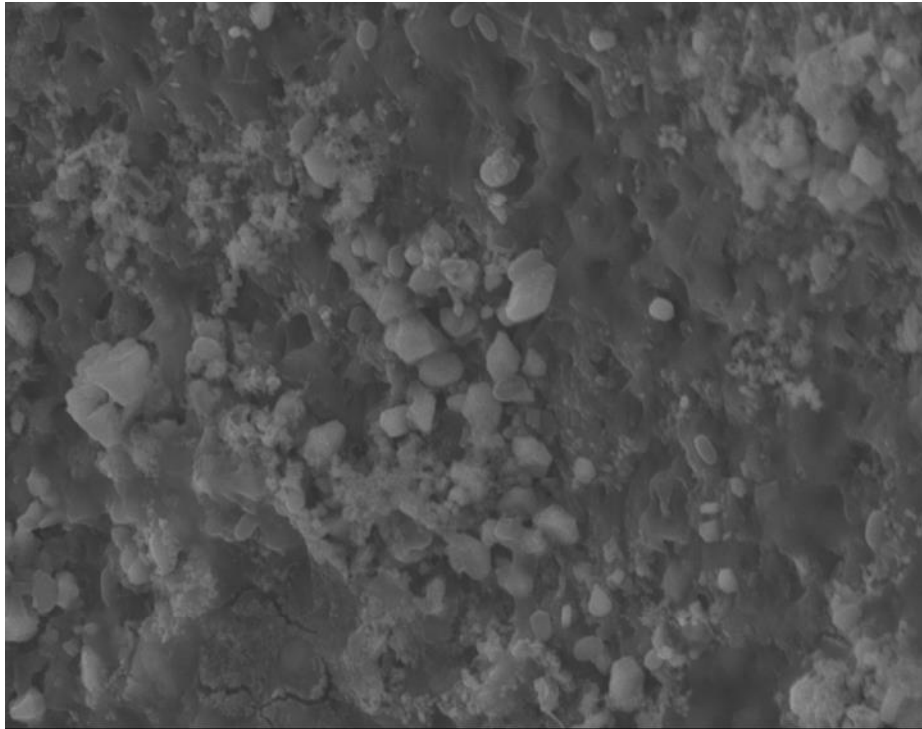


SED 20.0 kV WD 13.9 mm Std.-PC 60.0 HighVac. x3,000
STD 9572 June 15 2022




5 μ m

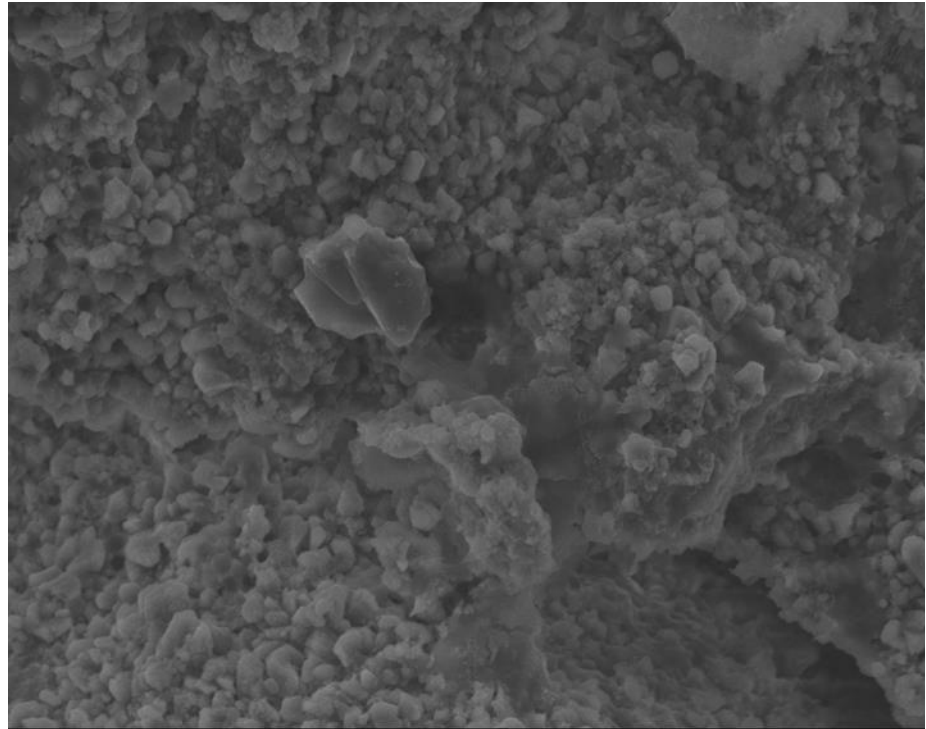


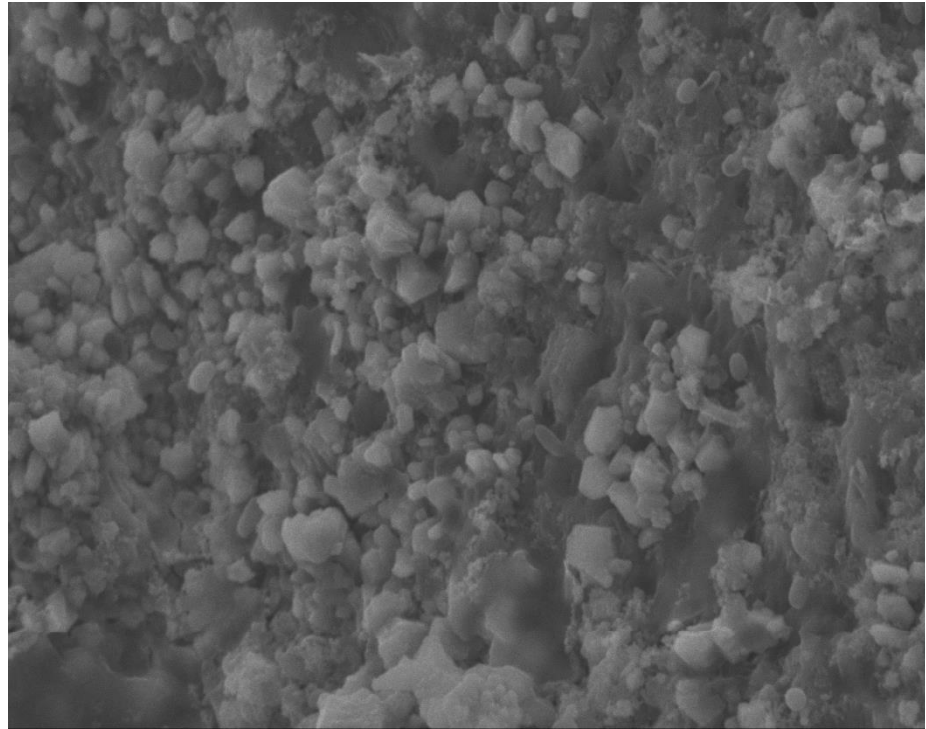
SED 20.0 kV WD 13.9 mm Std.-PC 60.0 HighVac. x1,700
STD 9573 June 15 2022




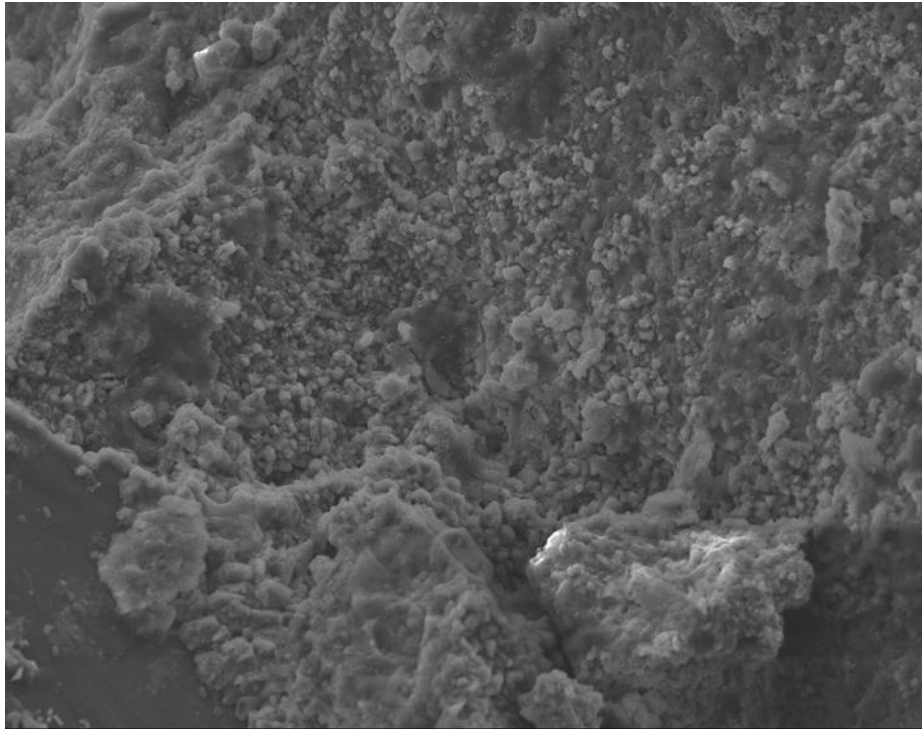
10 μ m

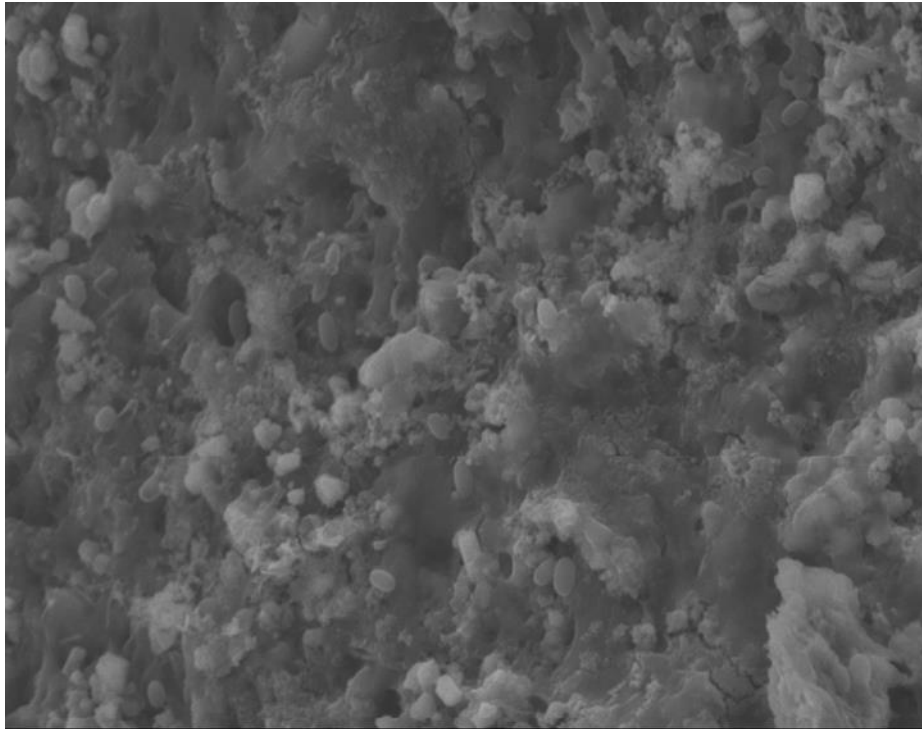


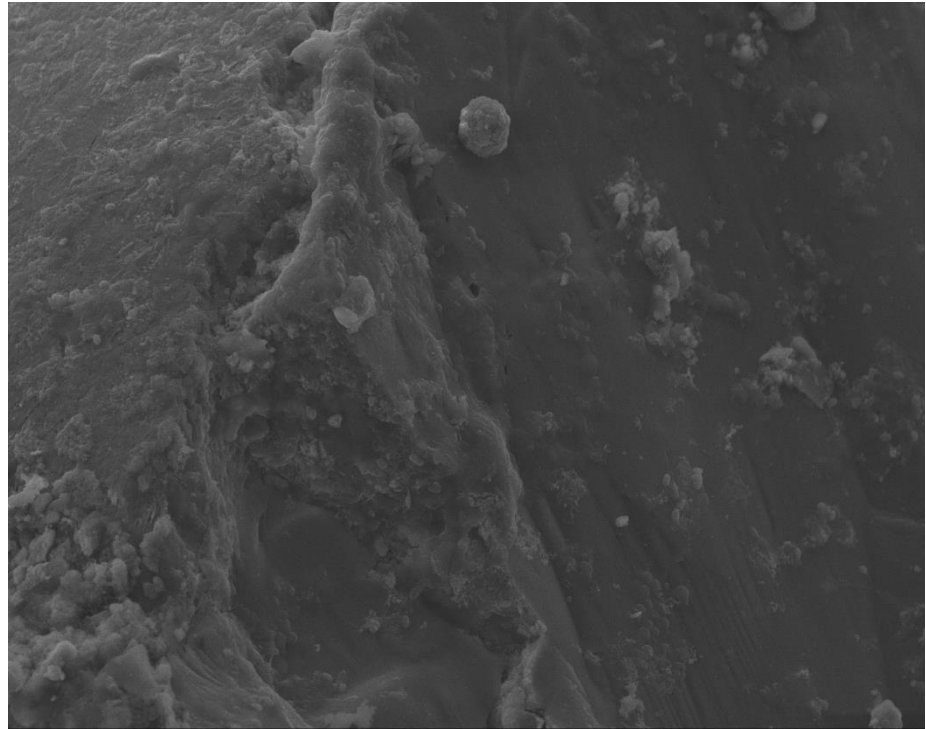
SED 20.0 kV WD 13.9 mm Std.-PC 60.0 HighVac. x3,000
STD 9571 June 15 2022




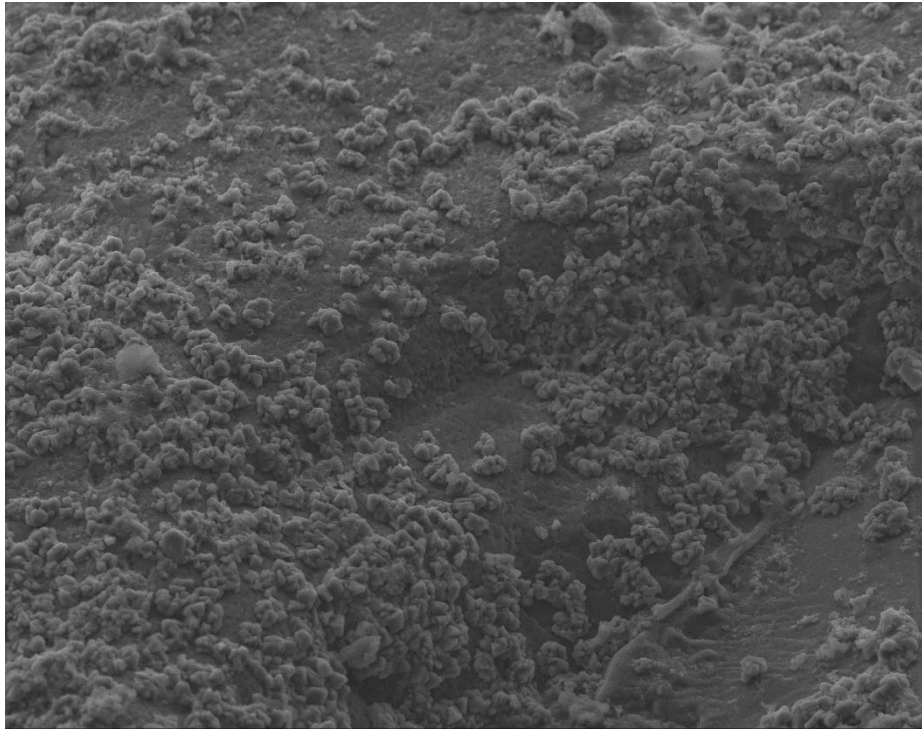
SED 20.0 kV WD 13.9 mm Std.-PC 60.0 HighVac. x3,000
STD 9570 June 15 2022






SED 20.0 kV WD 14.1 mm Std.-PC 60.0 HighVac. x900
STD 9569 June 15 2022






SED 20.0 kV WD 13.8 mm Std.-PC 60.0 HighVac. x1,000
STD 9567 June 15 2022

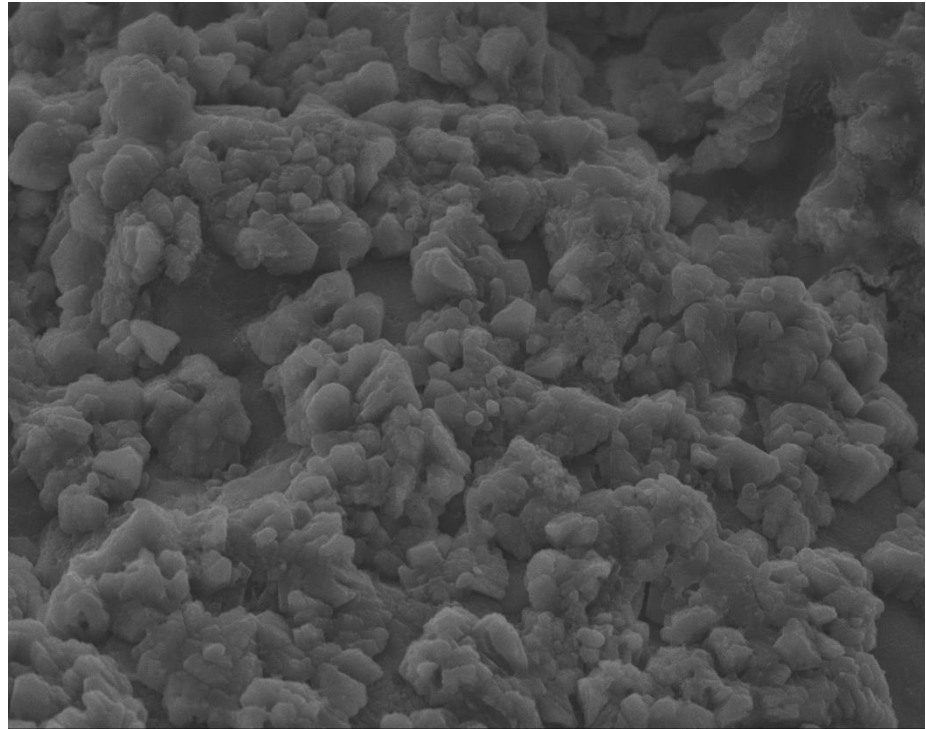


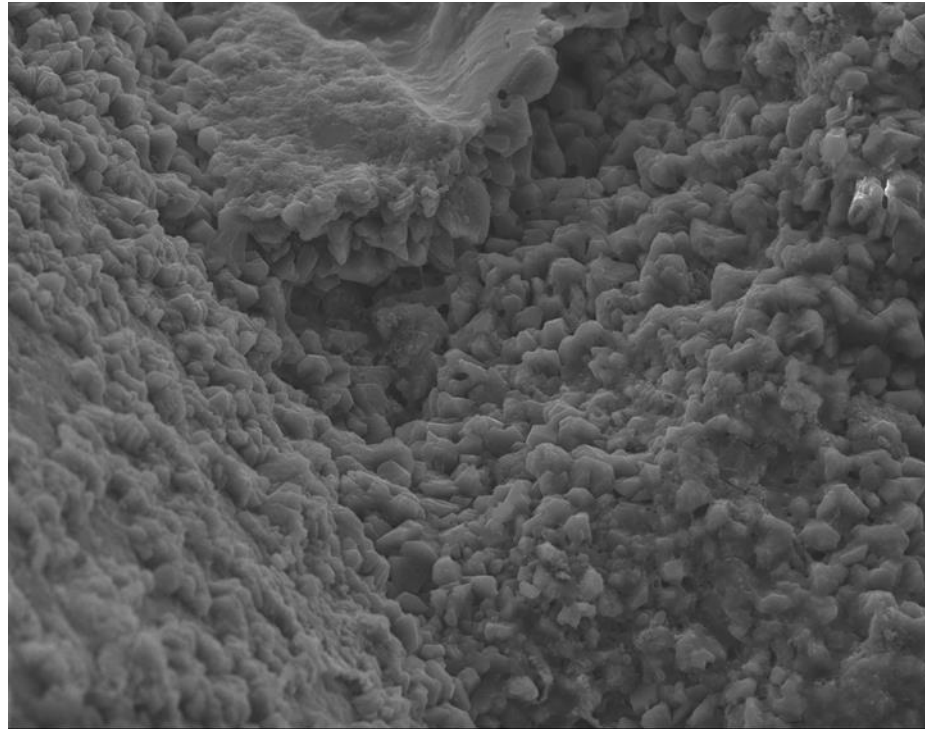
SED 20.0 kV WD 13.7 mm Std.-PC 60.0 HighVac. x500  50 μ m
STD 9566 June 15 2022




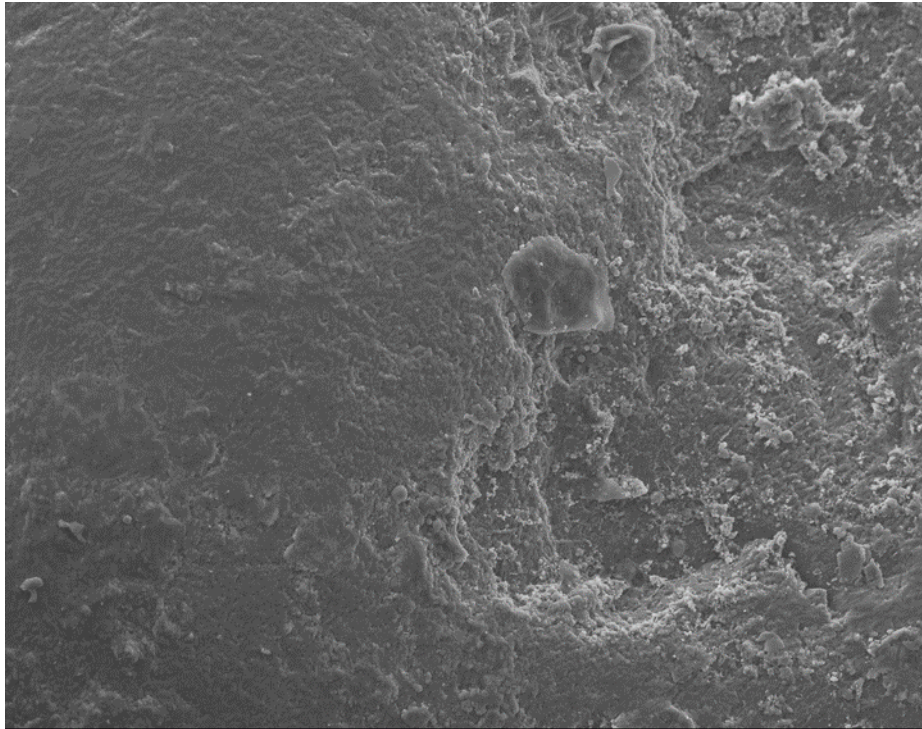
SED 20.0 kV WD 13.1 mm Std.-PC 60.0 HighVac. x2,000  10 μ m
STD 9565 June 15 2022

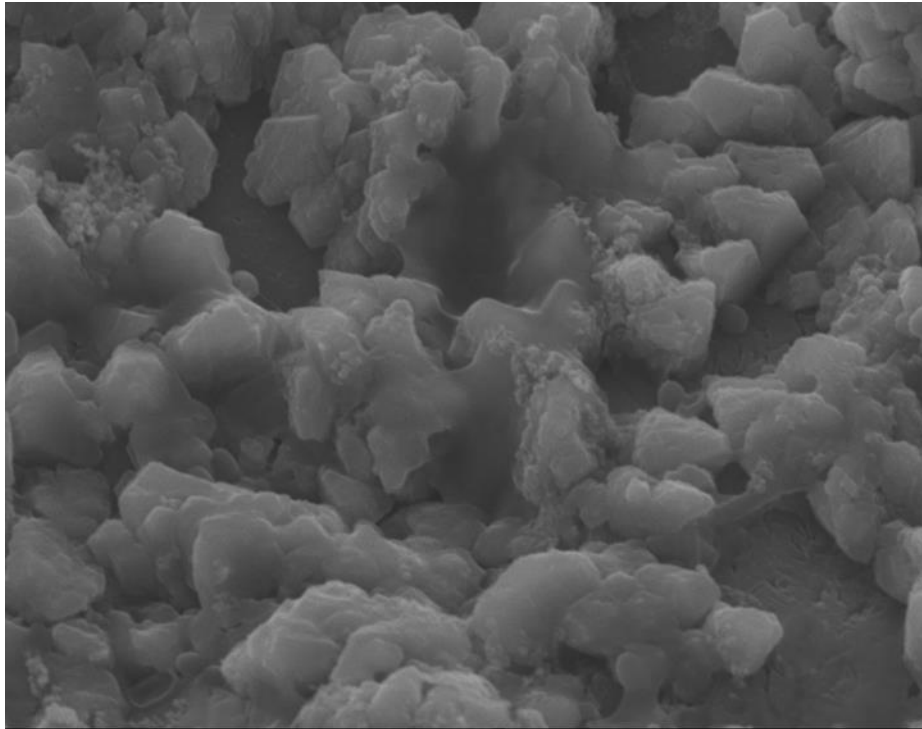


SED 20.0 kV WD 13.1 mm Std.-PC 60.0 HighVac. x4,000
STD 9564 June 15 2022




SED 20.0 kV WD 13.0 mm Std.-PC 60.0 HighVac. x1,000
STD 9563 June 15 2022






SED 20.0 kV WD 11.0 mm Std.-PC 80.0 HighVac. x500
STD 9481 June 10 2022 50 μm

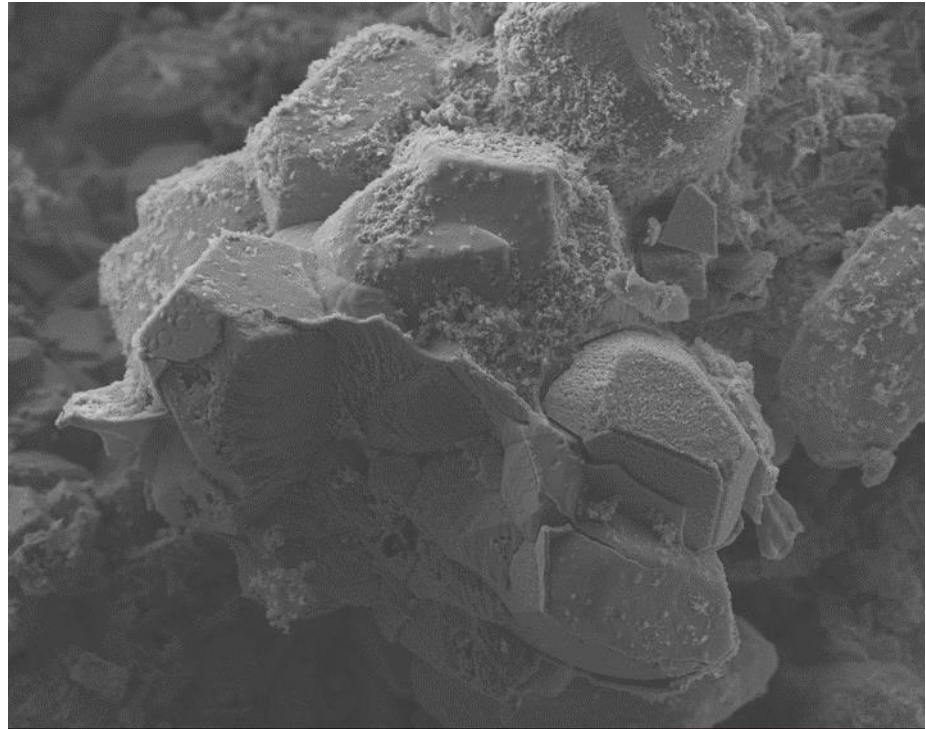

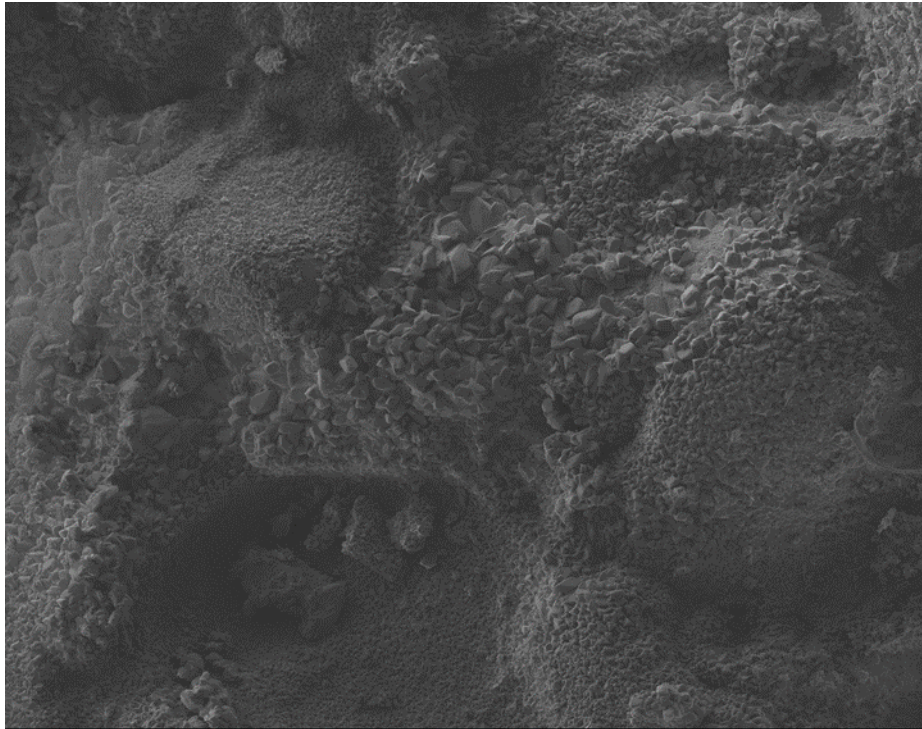

SED 20.0 kV WD 10.6 mm Std.-PC 60.0 HighVac. x500
STD 9480 June 10 2022 50 μm


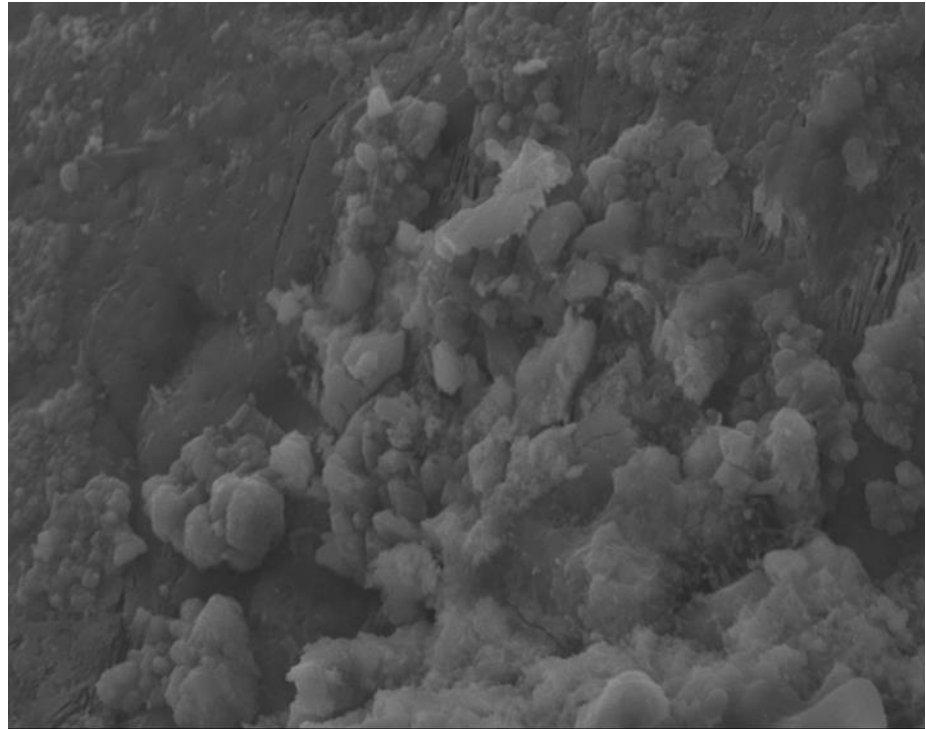



SED 20.0 kV WD 11.1 mm Std.-PC 80.0 HighVac. x50  500 μ m
STD 9482 June 10 2022




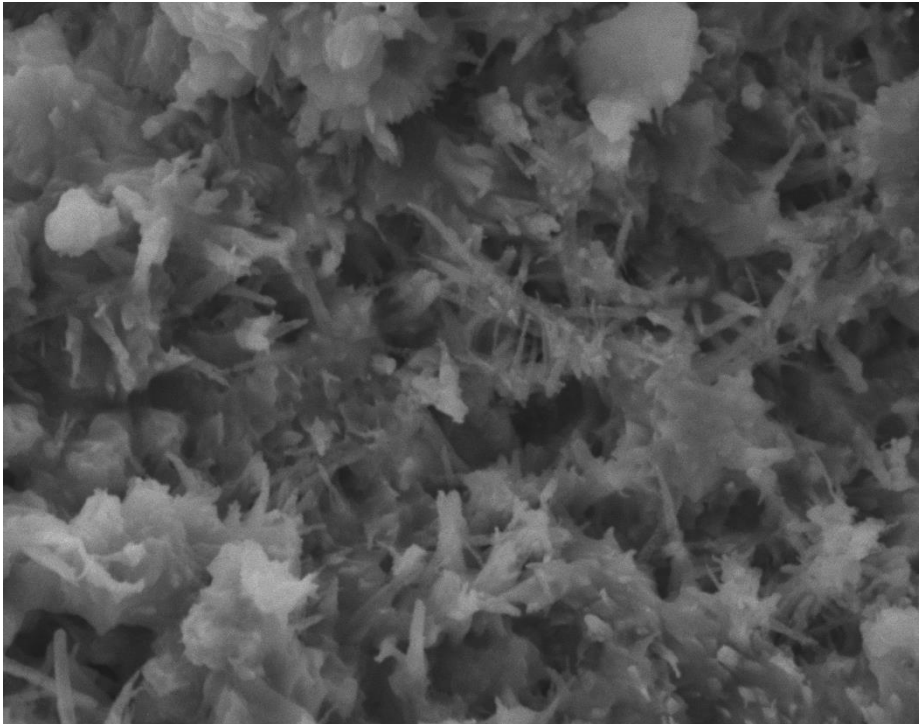
SED 20.0 kV WD 14.1 mm Std.-PC 60.0 HighVac. x3,000  5 μ m
STD 9568 June 15 2022


ΚΑΤΗΓΟΡΙΑ II (ΝΑΝΟΣΩΛΗΝΕΣ ΑΝΘΡΑΚΑ)

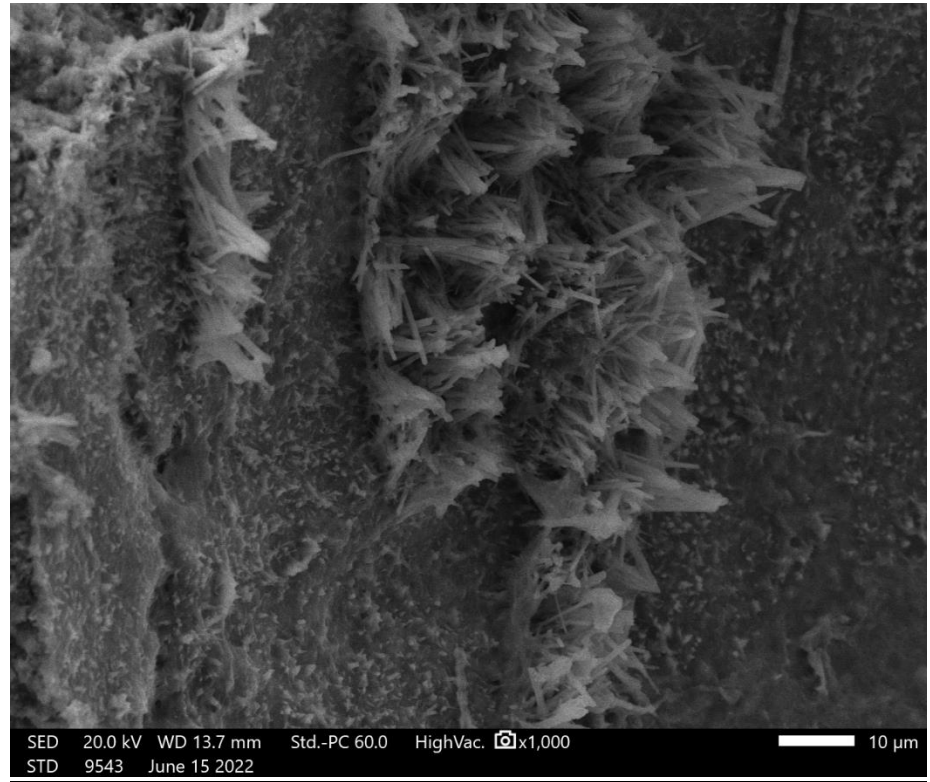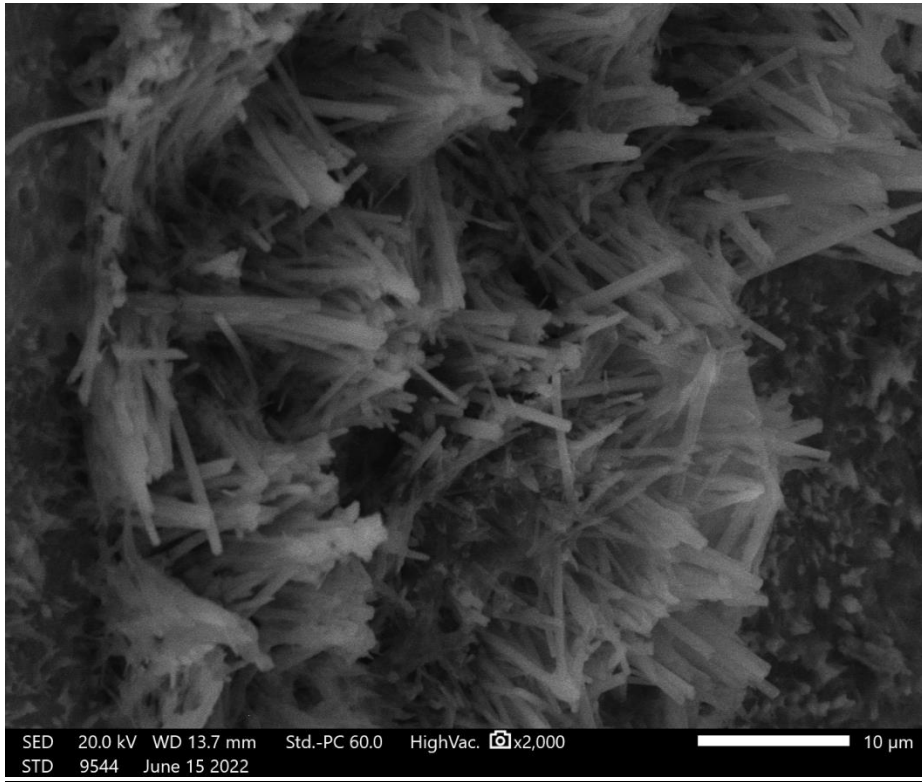


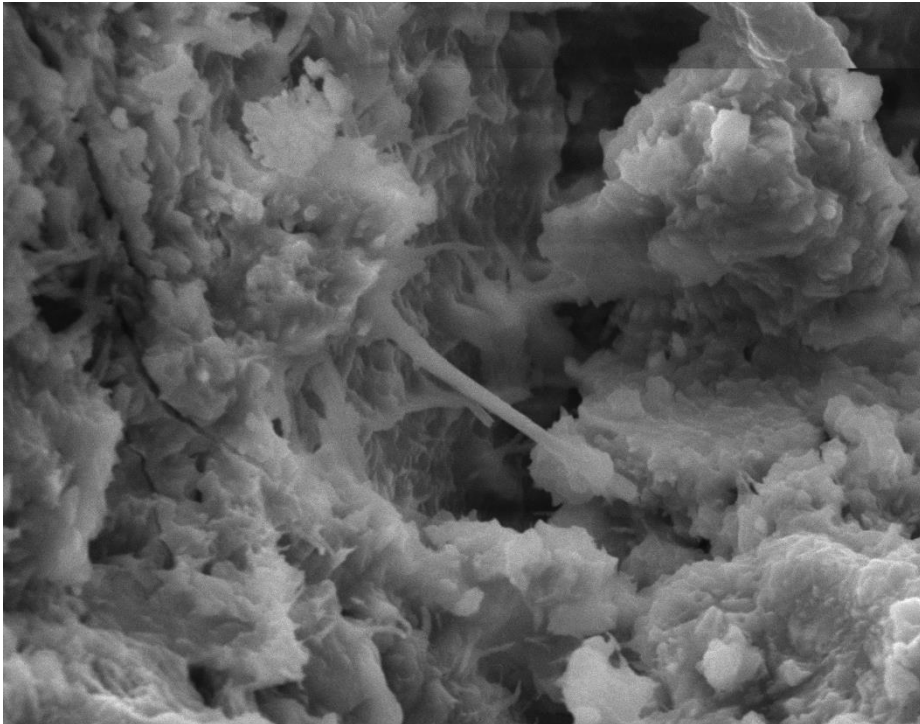




SED 20.0 kV WD 13.8 mm Std.-PC 60.0 HighVac. x3,000
STD 9541 June 15 2022



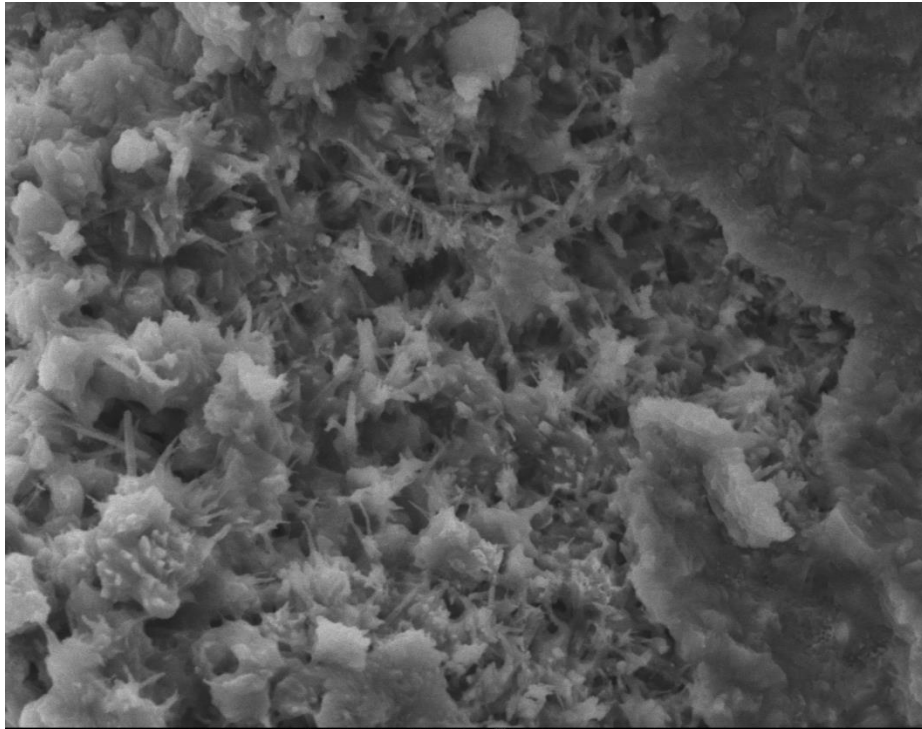


SED 20.0 kV WD 13.8 mm Std.-PC 60.0 HighVac. x4,000
STD 9540 June 15 2022



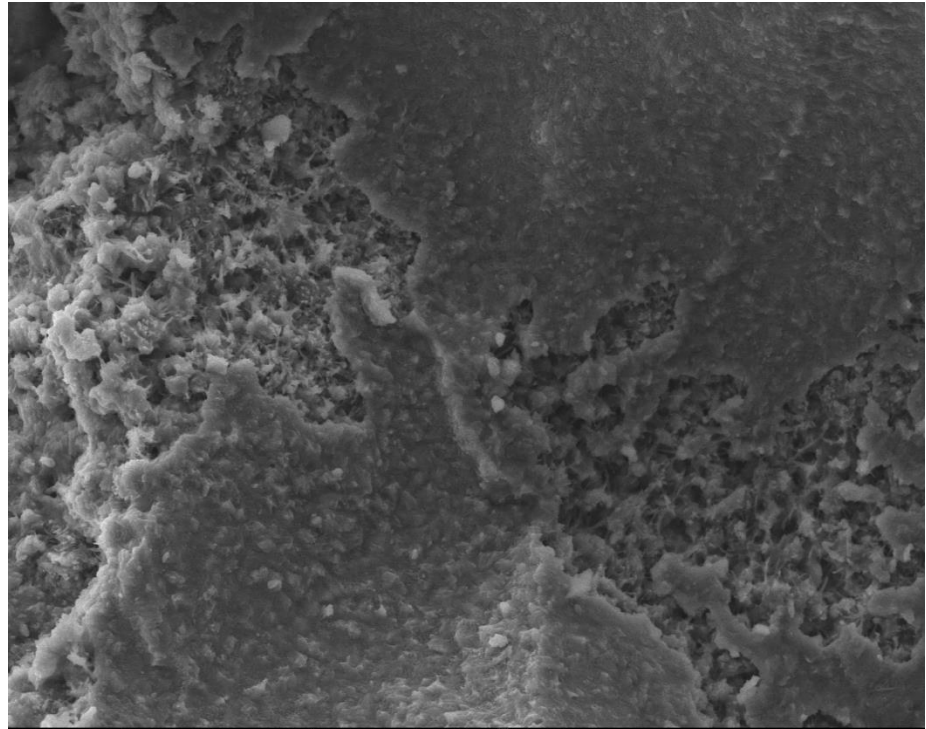


SED 20.0 kV WD 13.8 mm Std.-PC 60.0 HighVac. x2,500  10 μ m
STD 9538 June 15 2022



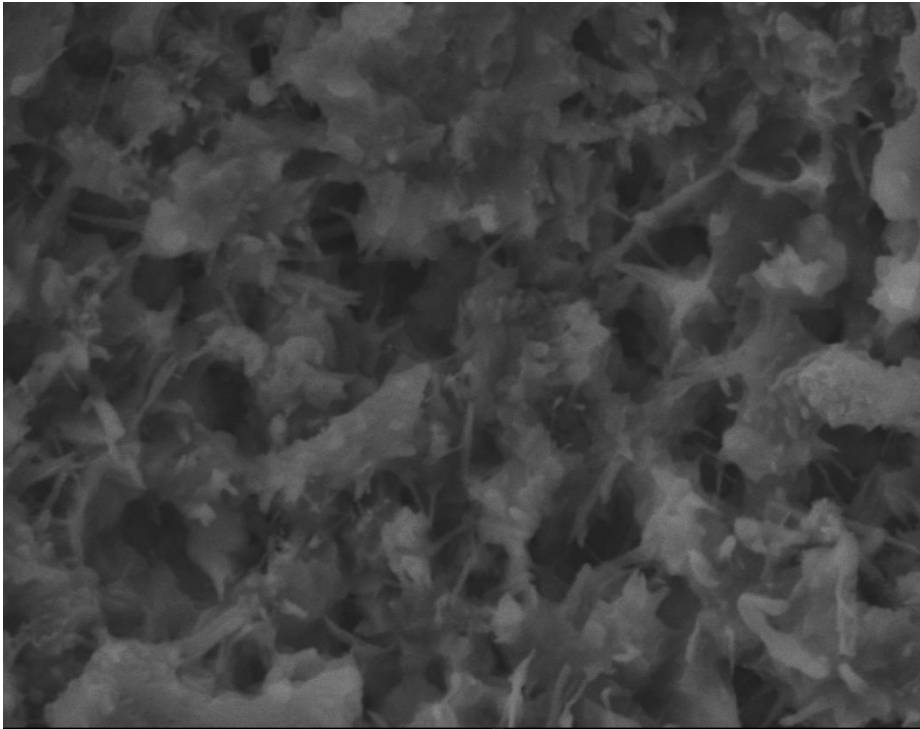


SED 20.0 kV WD 13.8 mm Std.-PC 60.0 HighVac. x1,000  10 μ m
STD 9537 June 15 2022

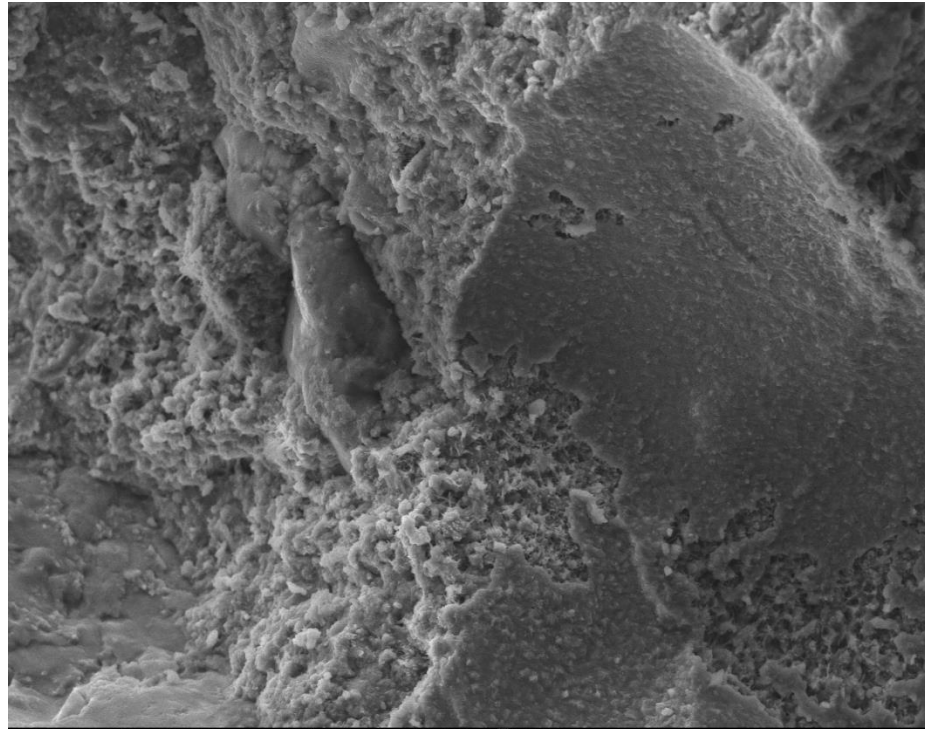


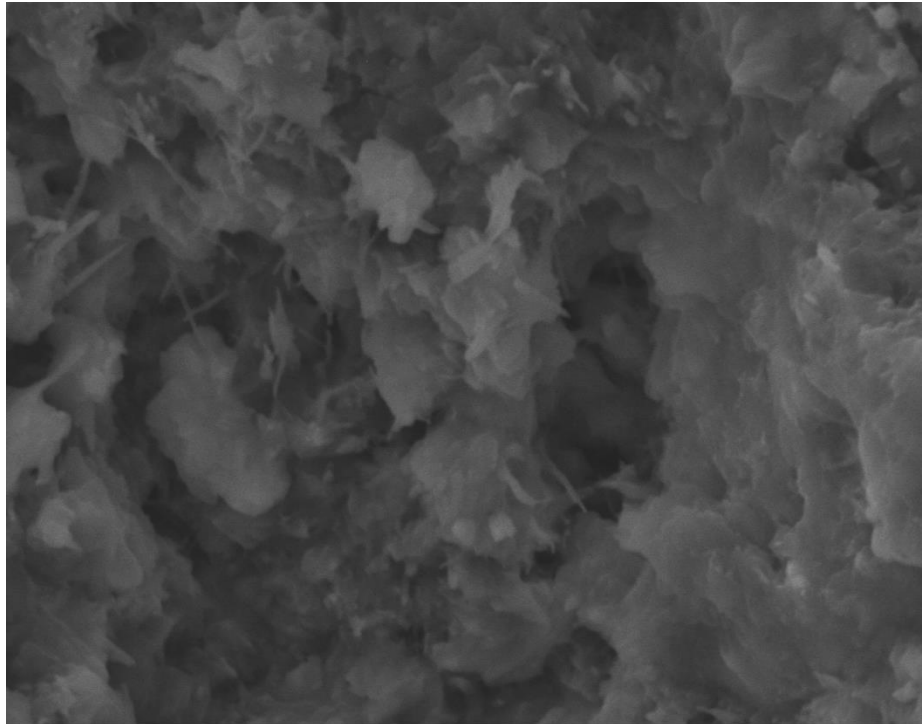
SED 20.0 kV WD 13.8 mm Std.-PC 60.0 HighVac. x4,000  5 μ m
STD 9535 June 15 2022




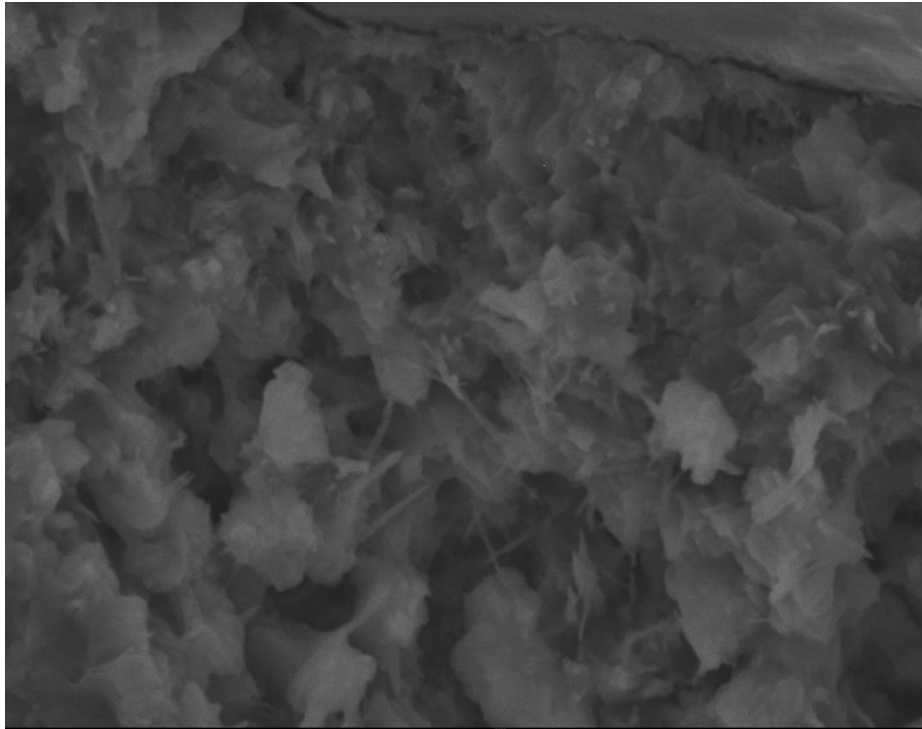
SED 20.0 kV WD 13.8 mm Std.-PC 60.0 HighVac. x600  20 μ m
STD 9536 June 15 2022

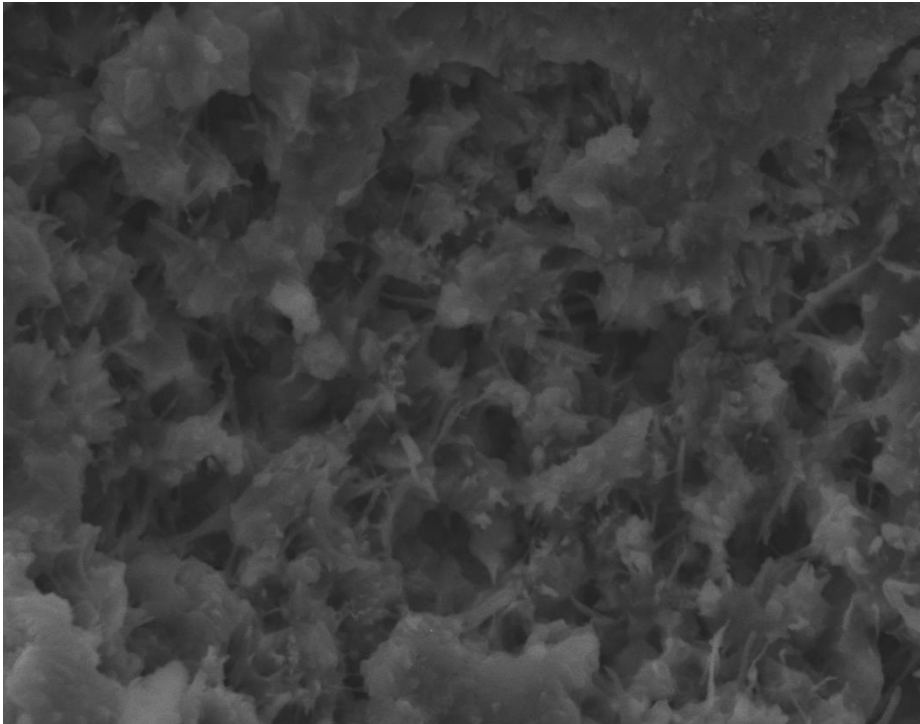




SED 20.0 kV WD 13.8 mm Std.-PC 60.0 HighVac. x3,000
STD 9534 June 15 2022






SED 20.0 kV WD 13.6 mm Std.-PC 60.0 HighVac. x4,000
STD 9533 June 15 2022



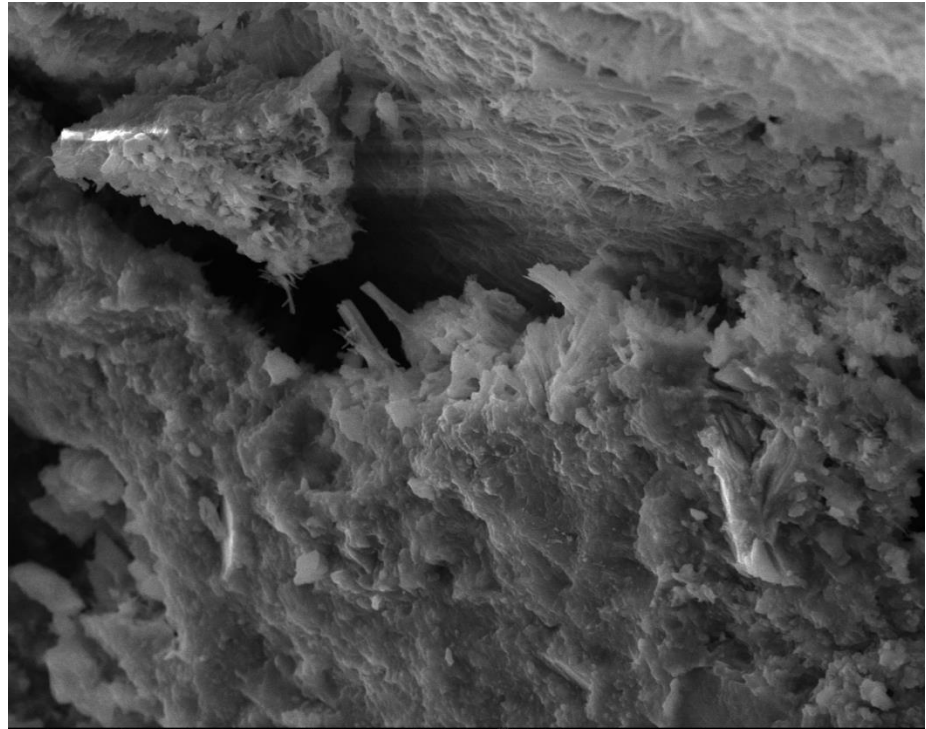


SED 20.0 kV WD 13.6 mm Std.-PC 60.0 HighVac. x4,000  5 μ m
STD 9532 June 15 2022



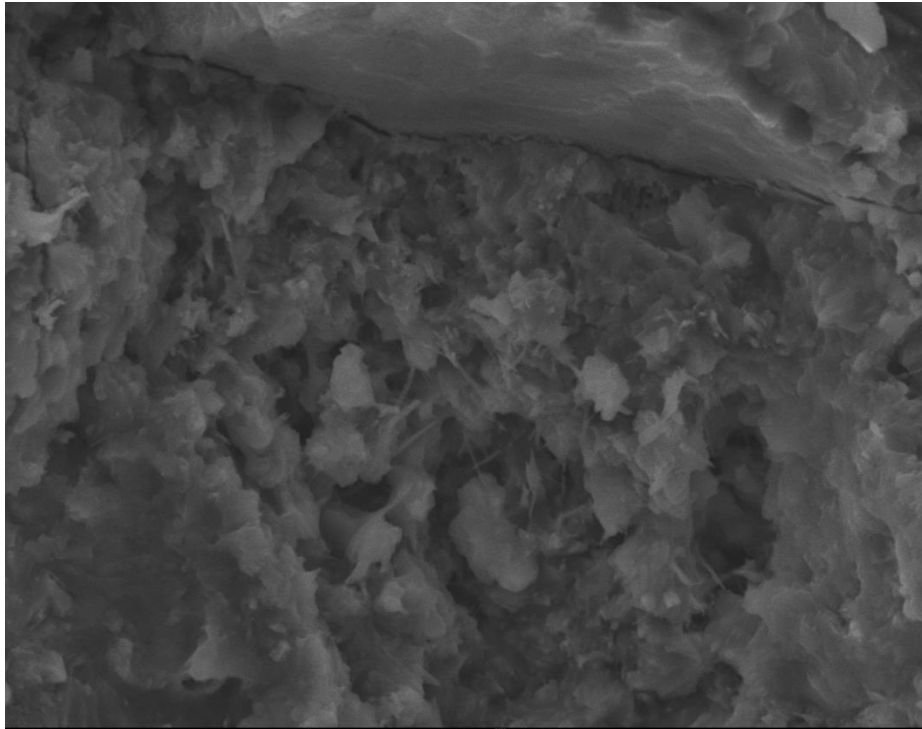


SED 20.0 kV WD 14.4 mm Std.-PC 60.0 HighVac. x1,500  10 μ m
STD 9530 June 15 2022

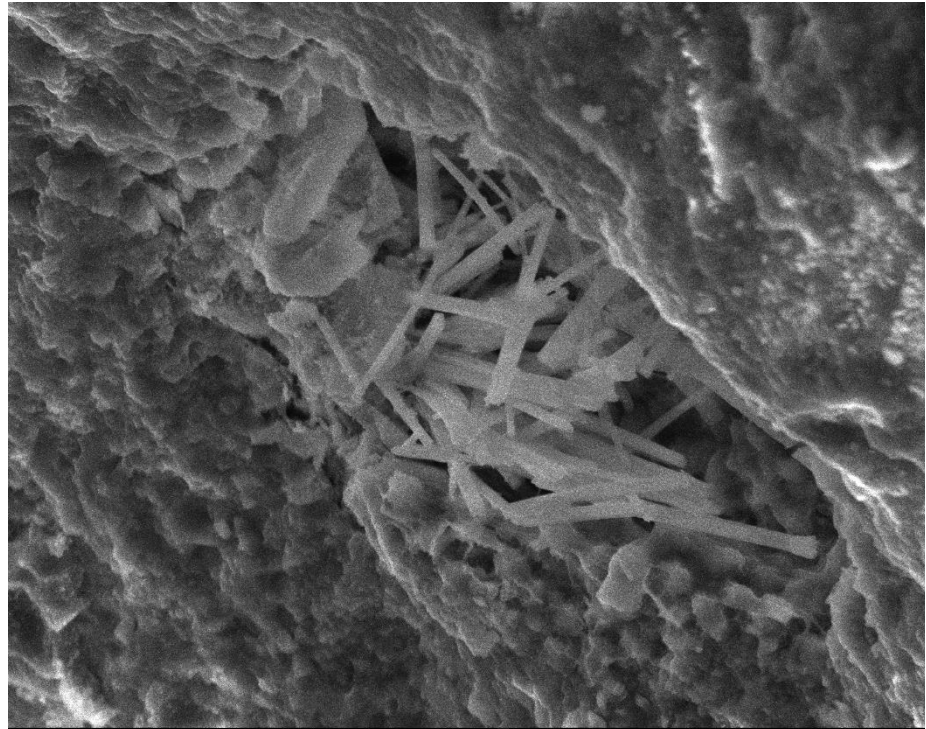


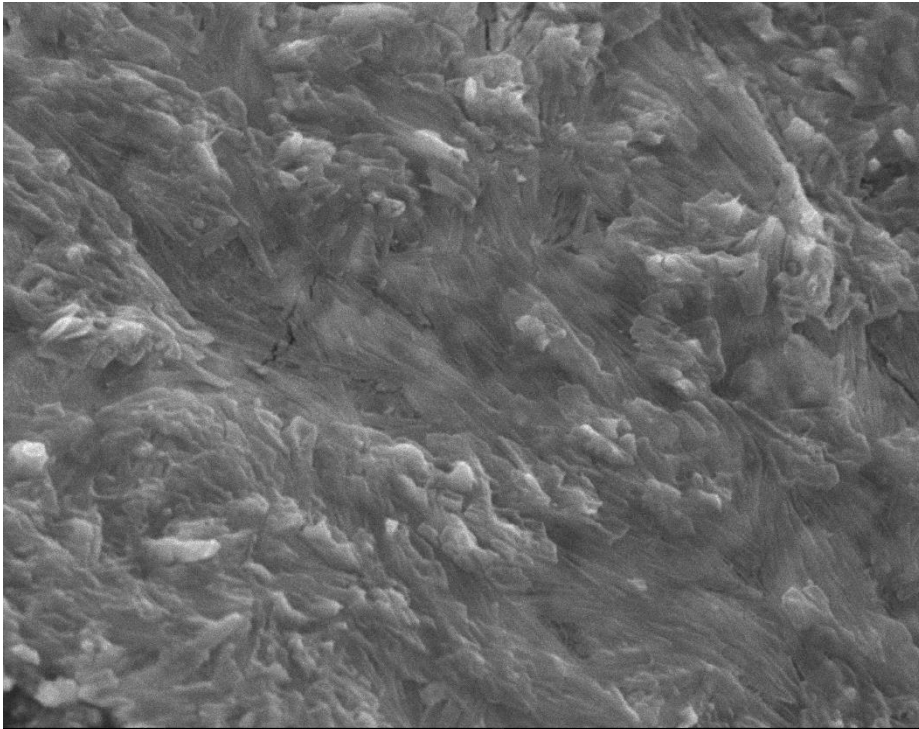
SED 20.0 kV WD 13.6 mm Std.-PC 60.0 HighVac. x2,500  10 μ m
STD 9531 June 15 2022




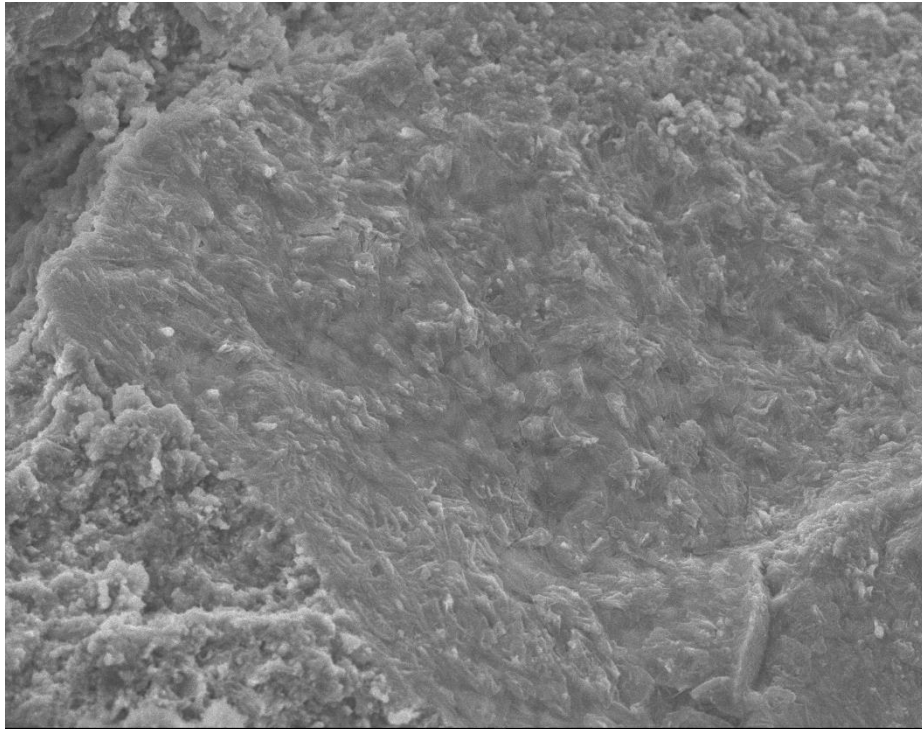
SED 20.0 kV WD 14.9 mm Std.-PC 40.0 HighVac. x2,000  10 μ m
STD 9522 June 14 2022

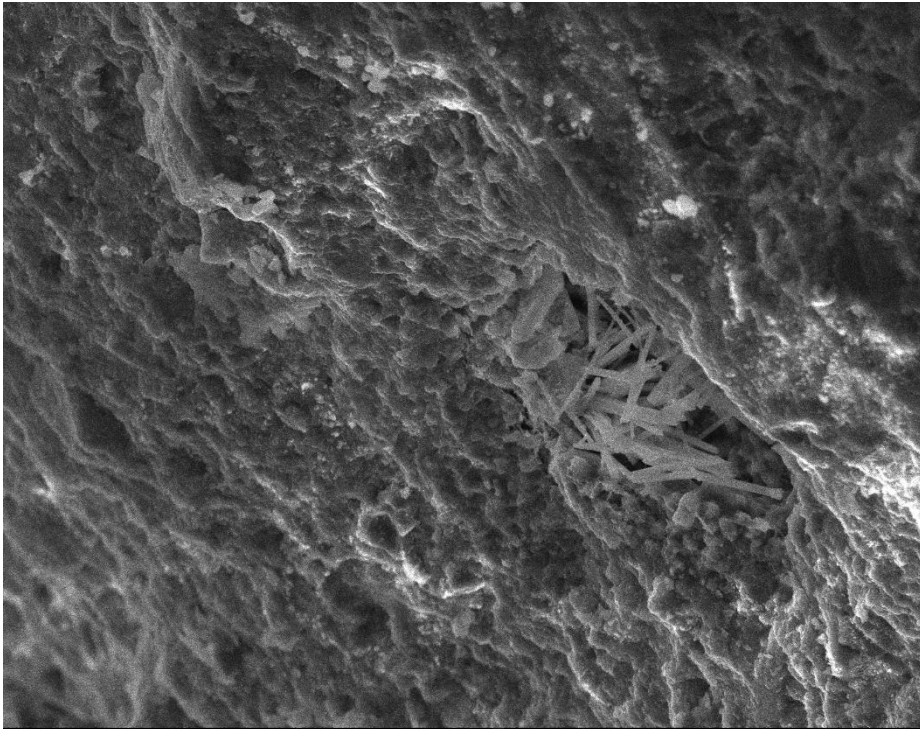




SED 20.0 kV WD 14.9 mm Std.-PC 40.0 HighVac. x1,000
STD 9521 June 14 2022





SED 20.0 kV WD 14.9 mm Std.-PC 60.0 HighVac. x3,000
STD 9519 June 14 2022


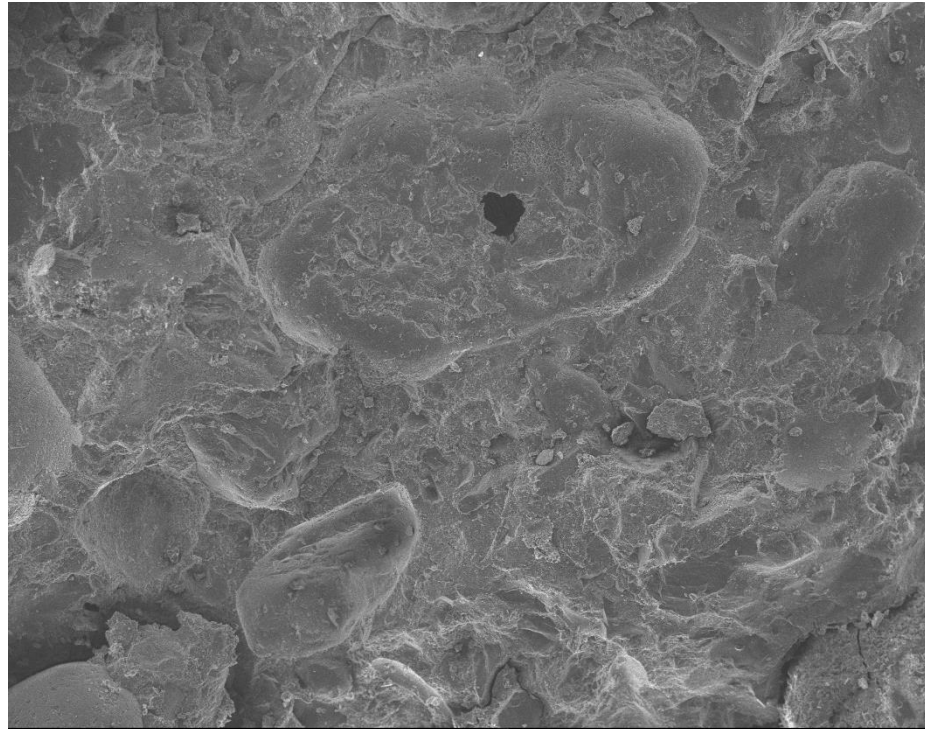



SED 20.0 kV WD 14.9 mm Std.-PC 60.0 HighVac. x1,000  10 μ m
STD 9518 June 14 2022






SED 20.0 kV WD 15.3 mm Std.-PC 60.0 HighVac. x40  500 μ m
STD 9517 June 14 2022

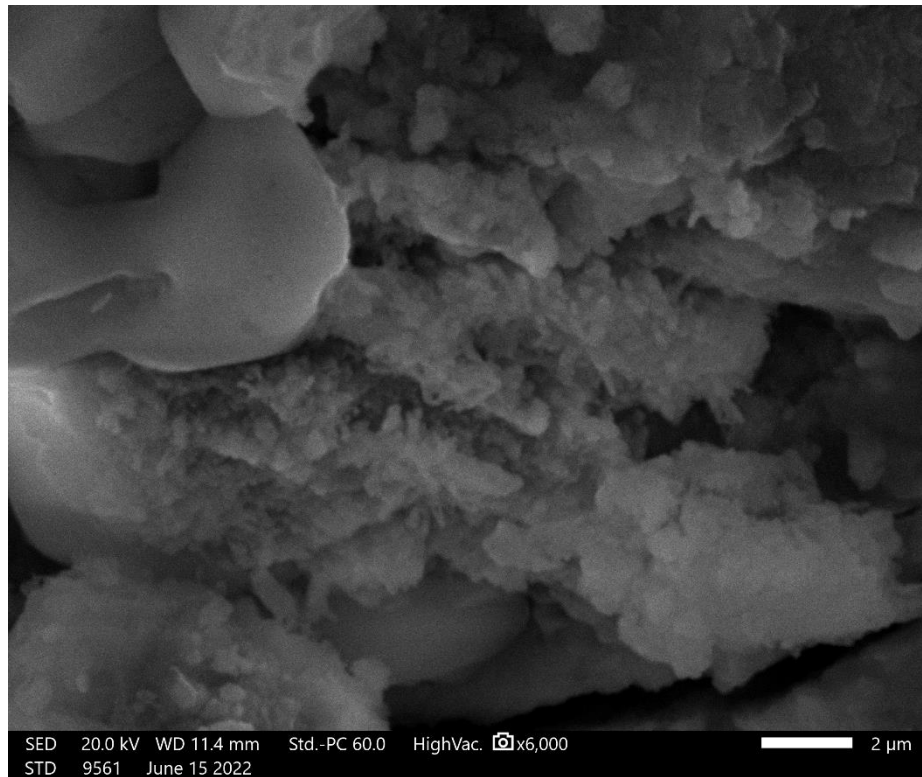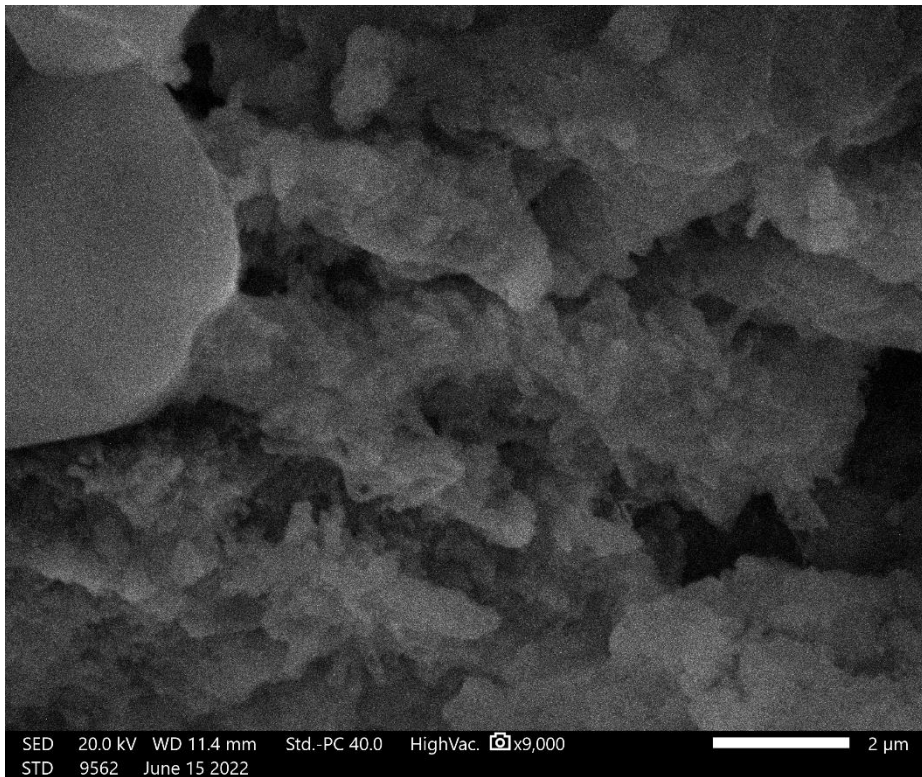

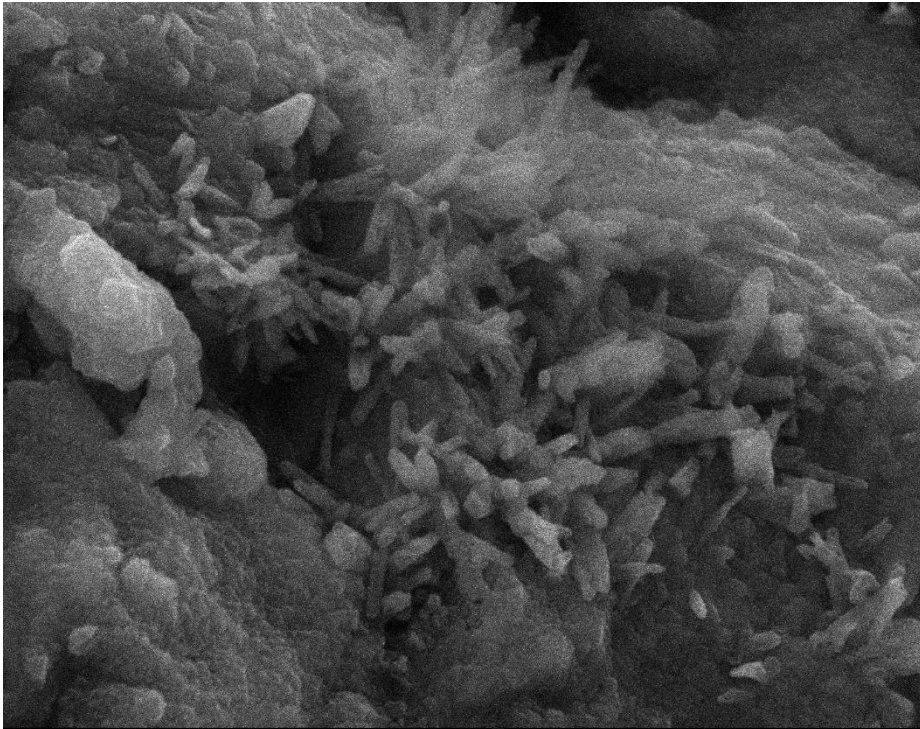ΚΑΤΗΓΟΡΙΑ III (ΝΑΝΟΪΝΕΣ ΑΝΘΡΑΚΑ)





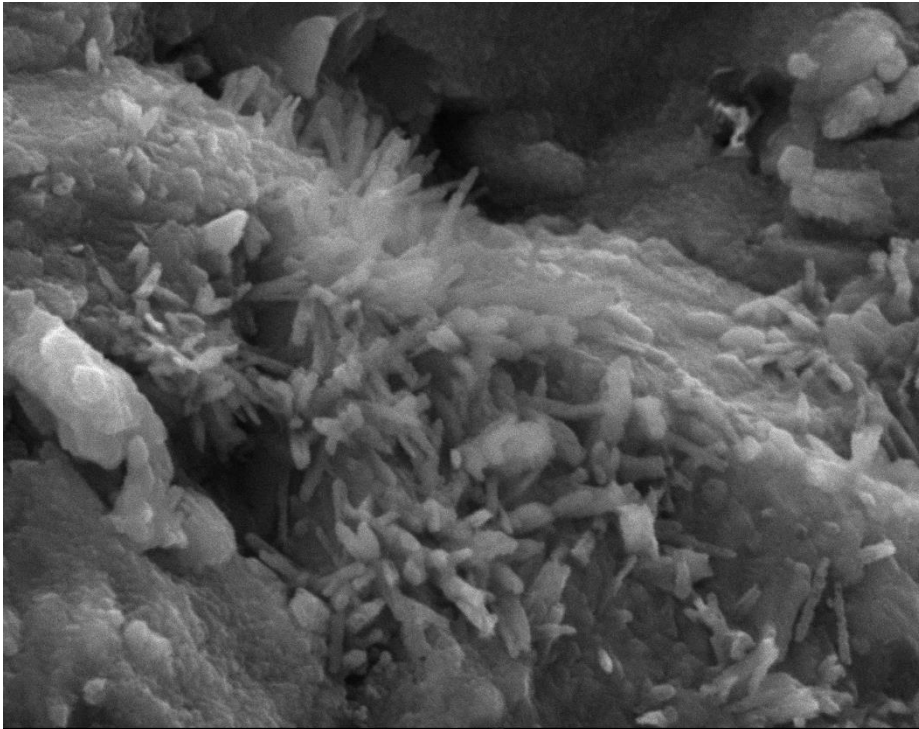



SED 20.0 kV WD 11.4 mm Std.-PC 40.0 HighVac. x6,000  2 μ m
STD 9560 June 15 2022





SED 20.0 kV WD 11.4 mm Std.-PC 60.0 HighVac. x5,000  5 μ m
STD 9559 June 15 2022

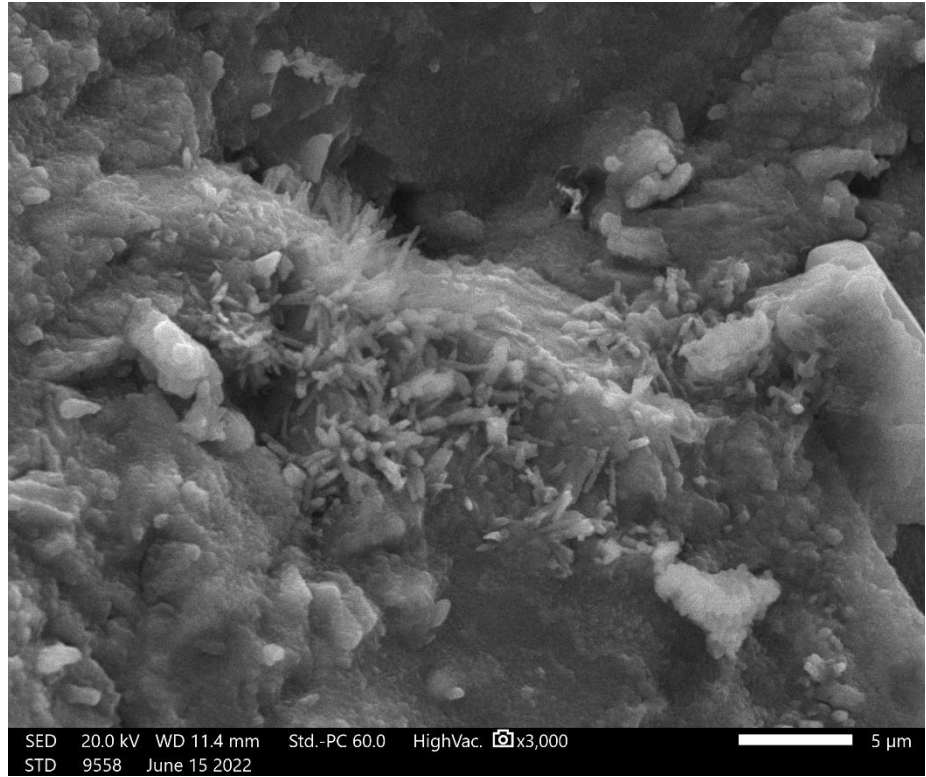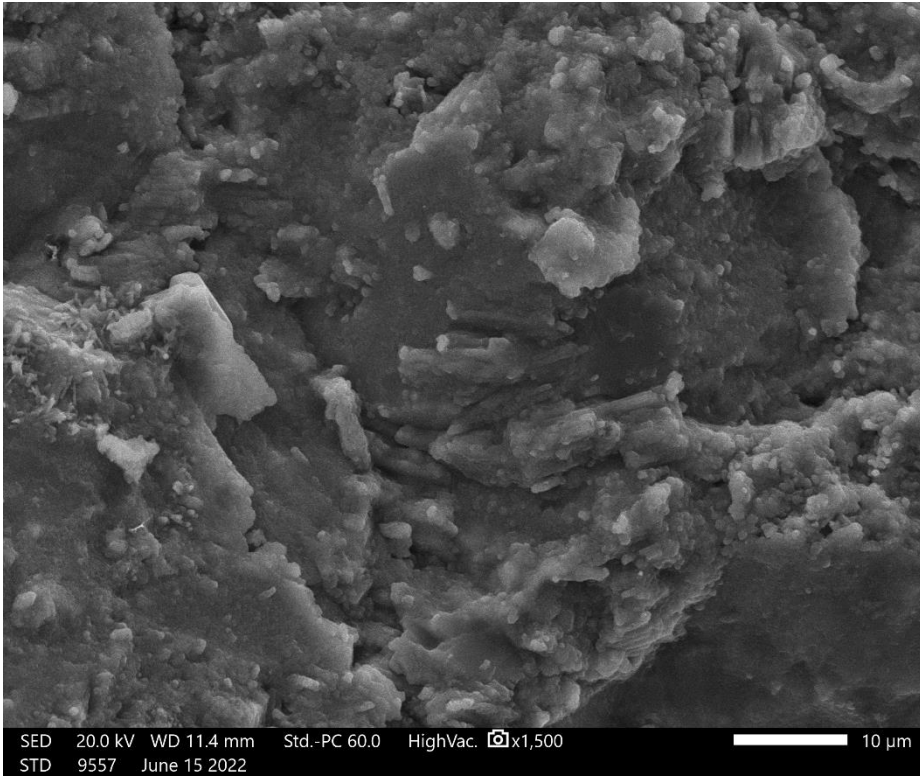


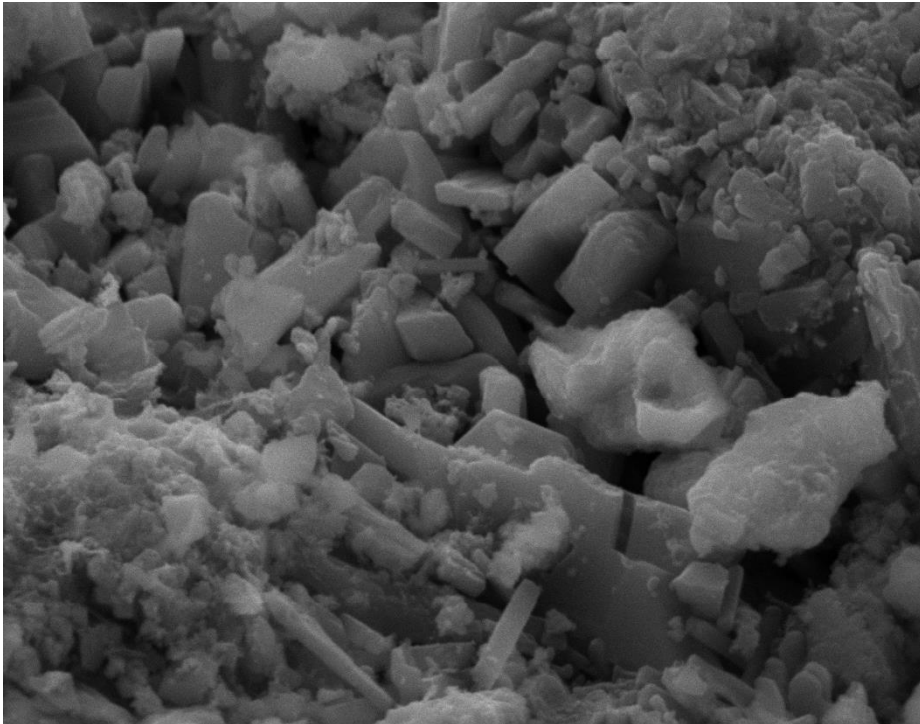


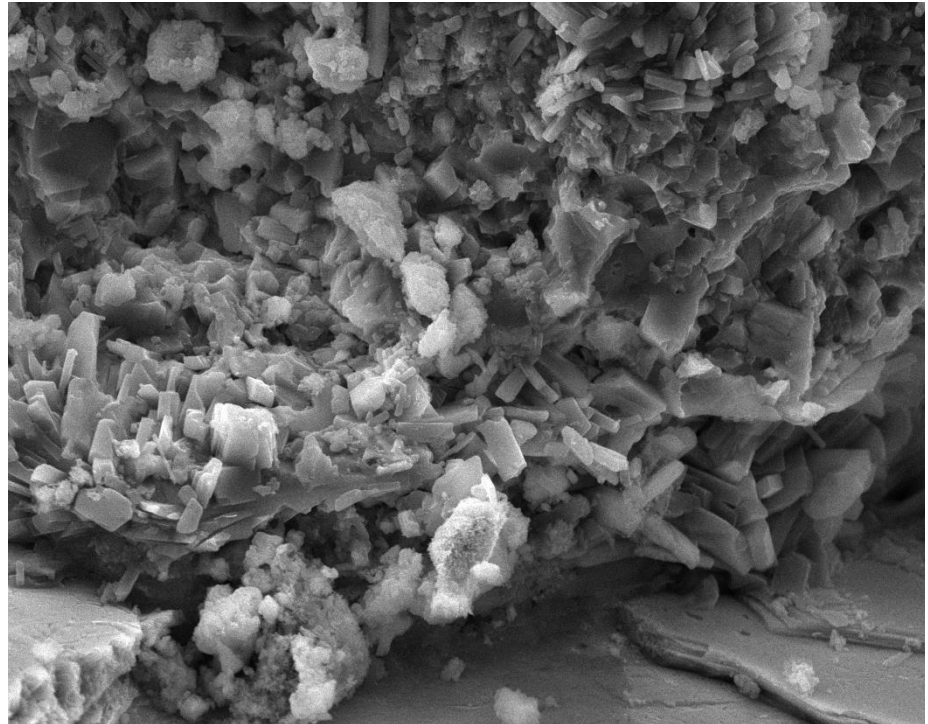
SED 20.0 kV WD 11.1 mm Std.-PC 60.0 HighVac. x4,000
STD 9556 June 15 2022

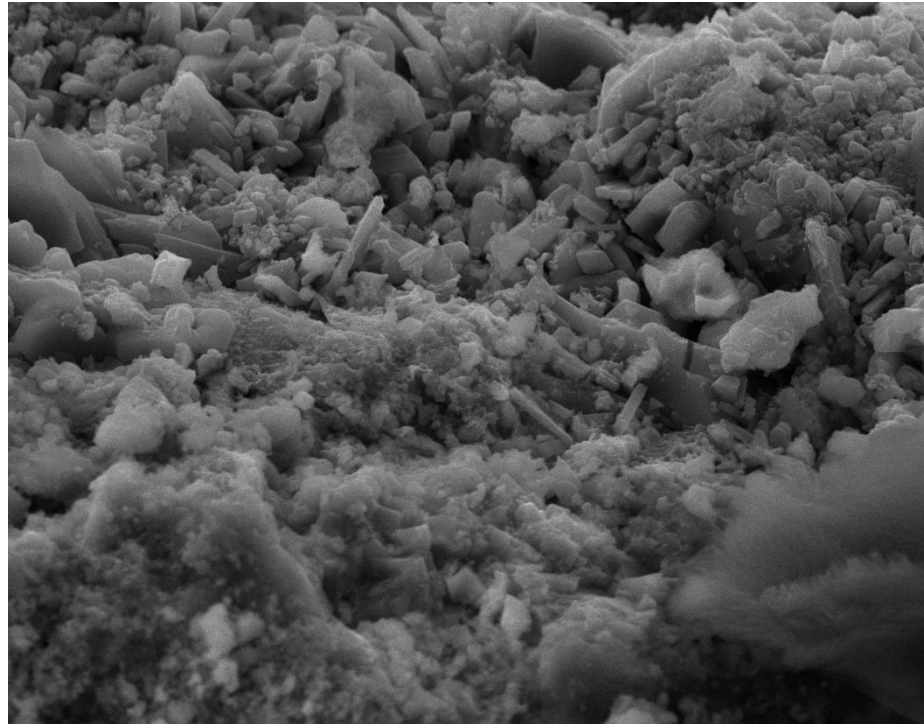


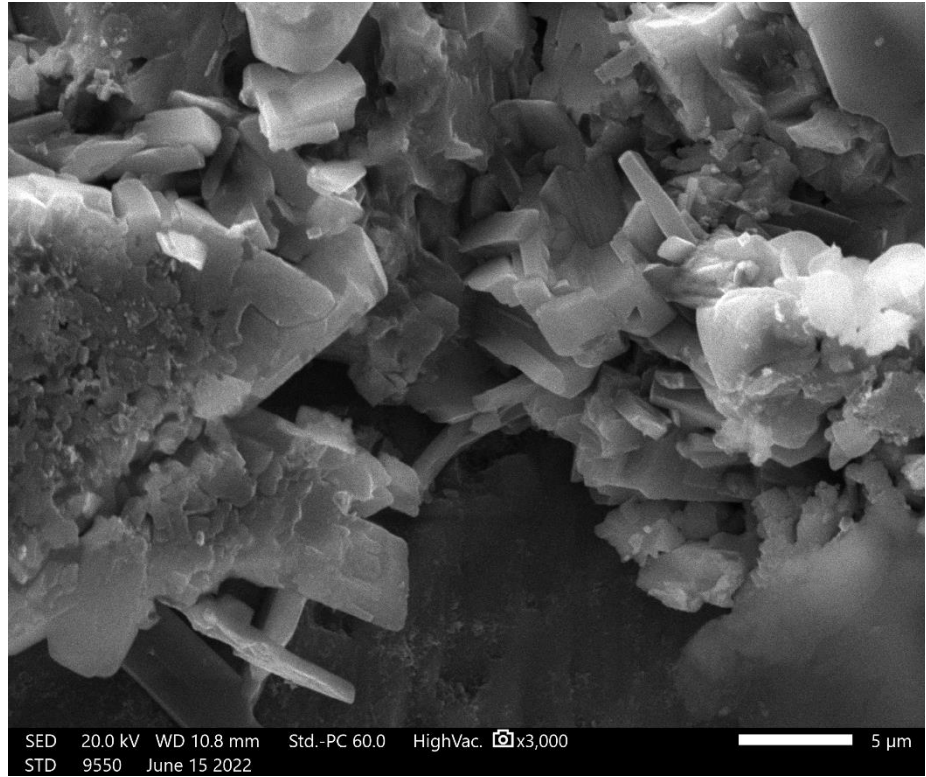
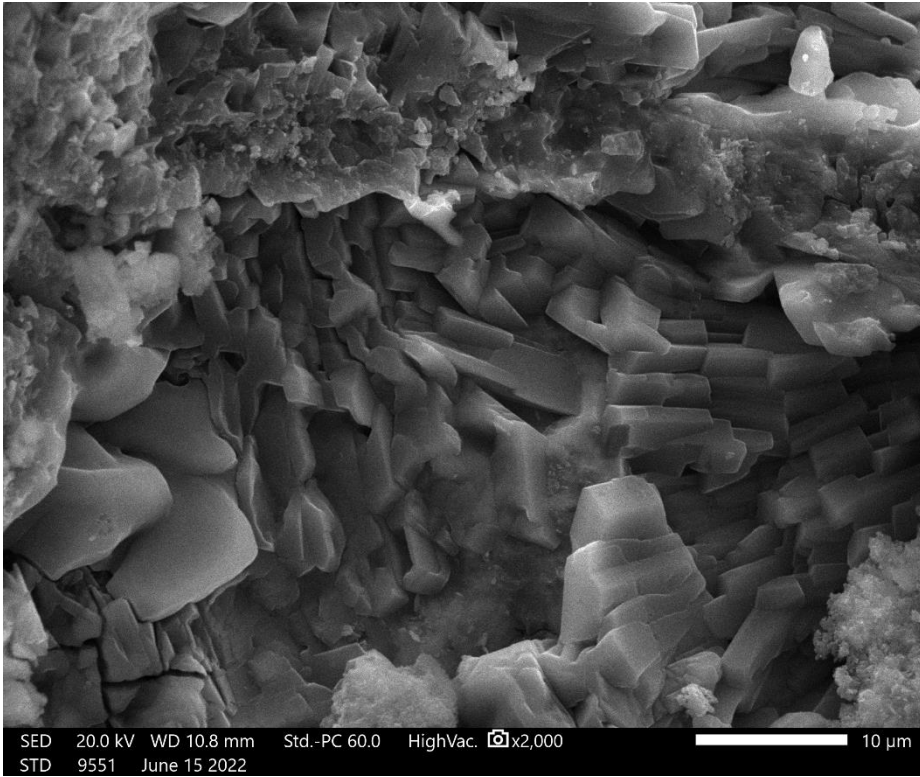
SED 20.0 kV WD 11.1 mm Std.-PC 60.0 HighVac. x2,000
STD 9555 June 15 2022

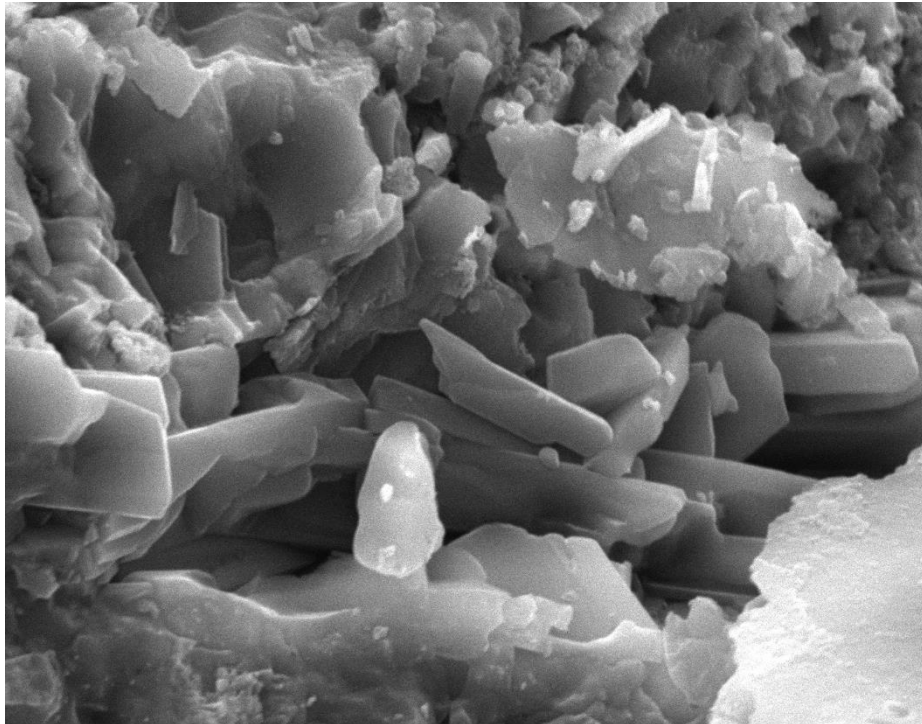



SED 20.0 kV WD 10.9 mm Std.-PC 60.0 HighVac. x4,000
STD 9552 June 15 2022 5 μ m





SED 20.0 kV WD 11.0 mm Std.-PC 60.0 HighVac. x1,600
STD 9554 June 15 2022 10 μ m




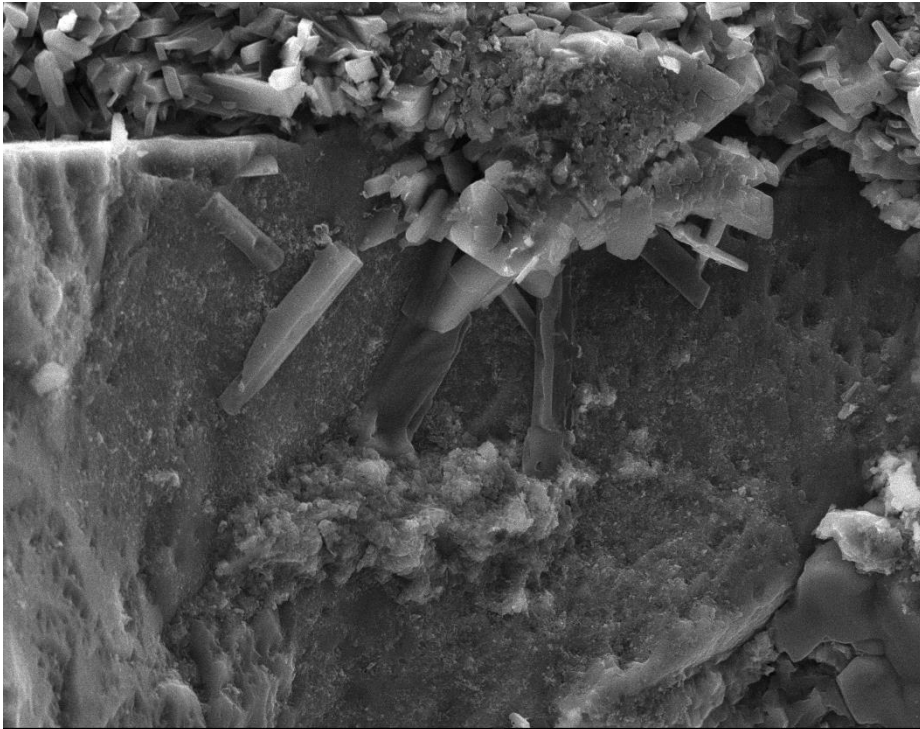


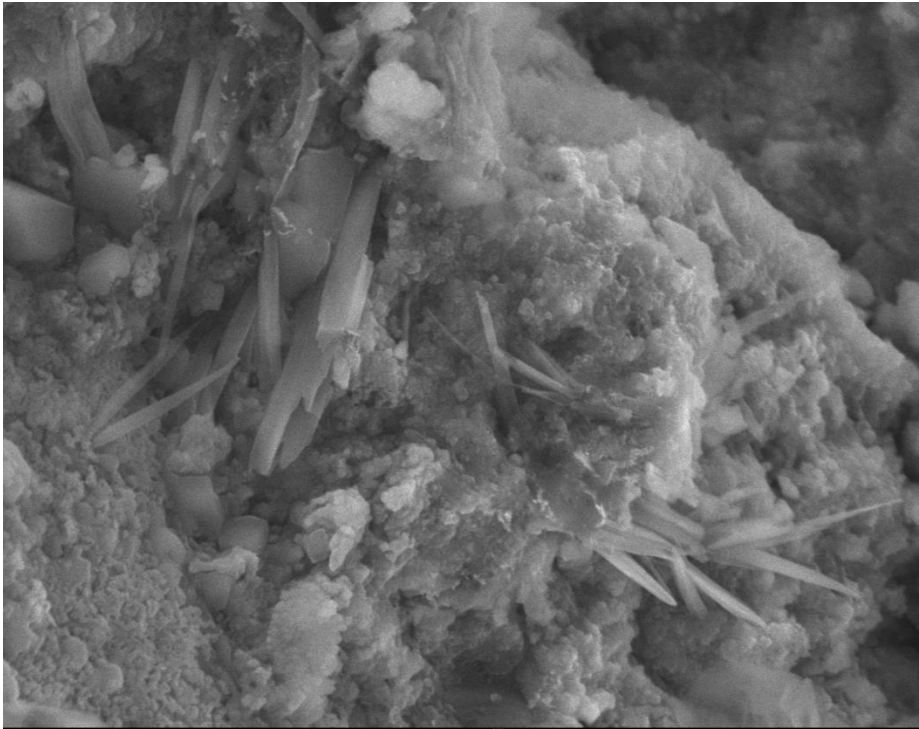
SED 20.0 kV WD 10.8 mm Std.-PC 60.0 HighVac. x1,400
STD 9549 June 15 2022

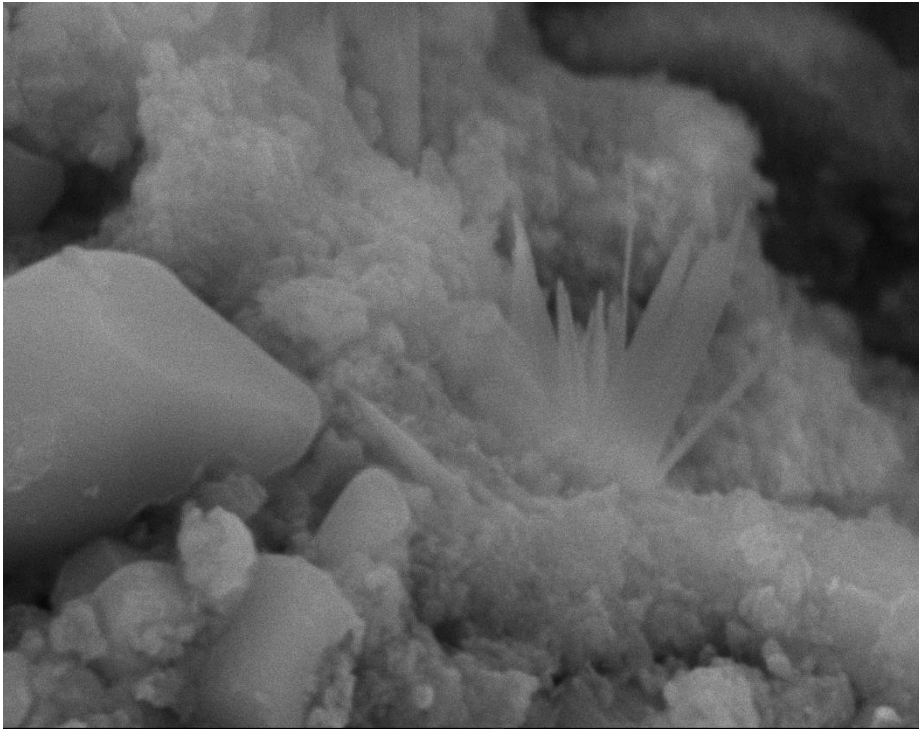


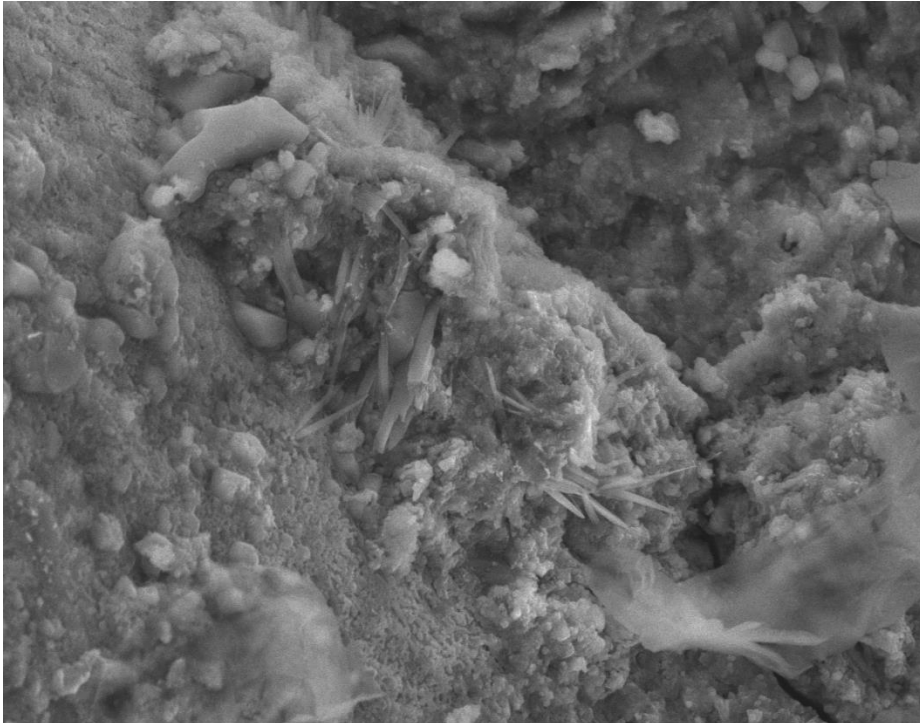
SED 20.0 kV WD 10.9 mm Std.-PC 60.0 HighVac. x7,000
STD 9548 June 15 2022

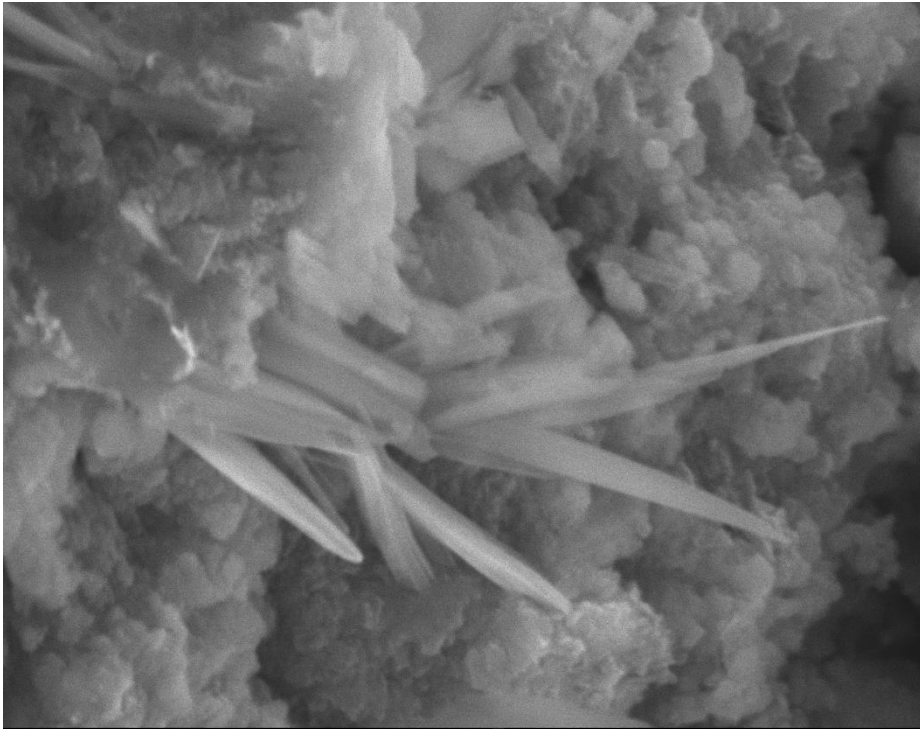


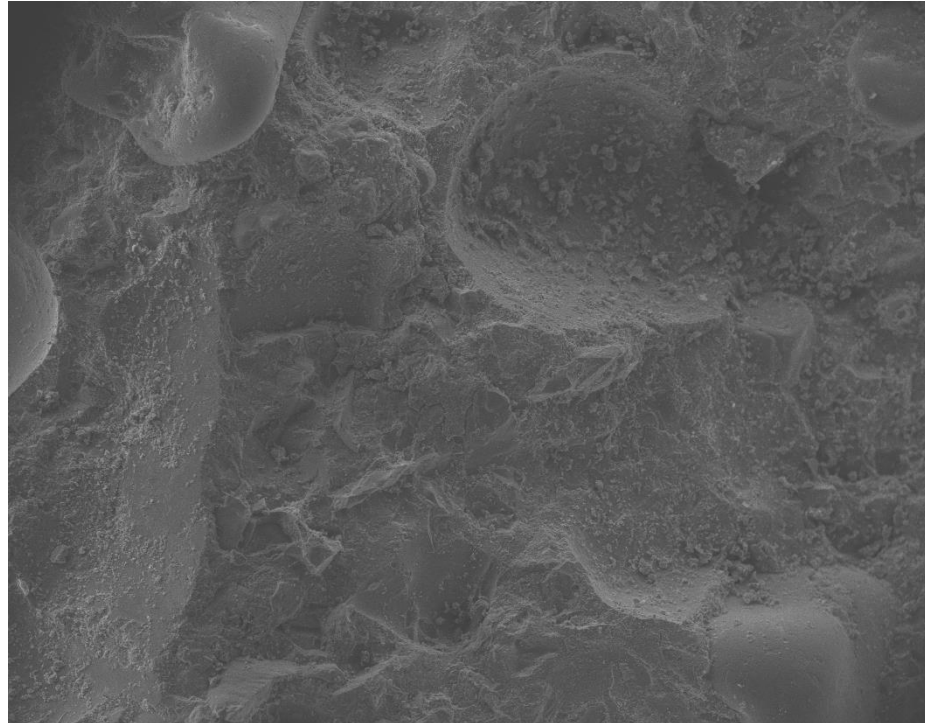
SED 20.0 kV WD 10.9 mm Std.-PC 60.0 HighVac. x7,000
STD 9547 June 15 2022




SED 20.0 kV WD 10.9 mm Std.-PC 60.0 HighVac. x3,000
STD 9546 June 15 2022



SED 20.0 kV WD 10.8 mm Std.-PC 60.0 HighVac. x1,500
STD 9545 June 15 2022



SED 20.0 kV WD 11.4 mm Std.-PC 60.0 HighVac. x40
STD 9515 June 14 2022